

Automatické biochemické analyzátory

Automatic
Analyzer V.E. 1141-0

HITACHI





AK22
AK22

101 102 103

R1

201 202 203


A CAUTION
Keep cover closed during operation


Väljnings komrvärde
CB R1 R2
MG R1
KREA R1
CA R1

Do not operate this instrument unless you have been trained and authorized to do so. For more information, see the user manual.

WARNING
Do not operate this instrument unless you have been trained and authorized to do so. For more information, see the user manual.

D EF IS

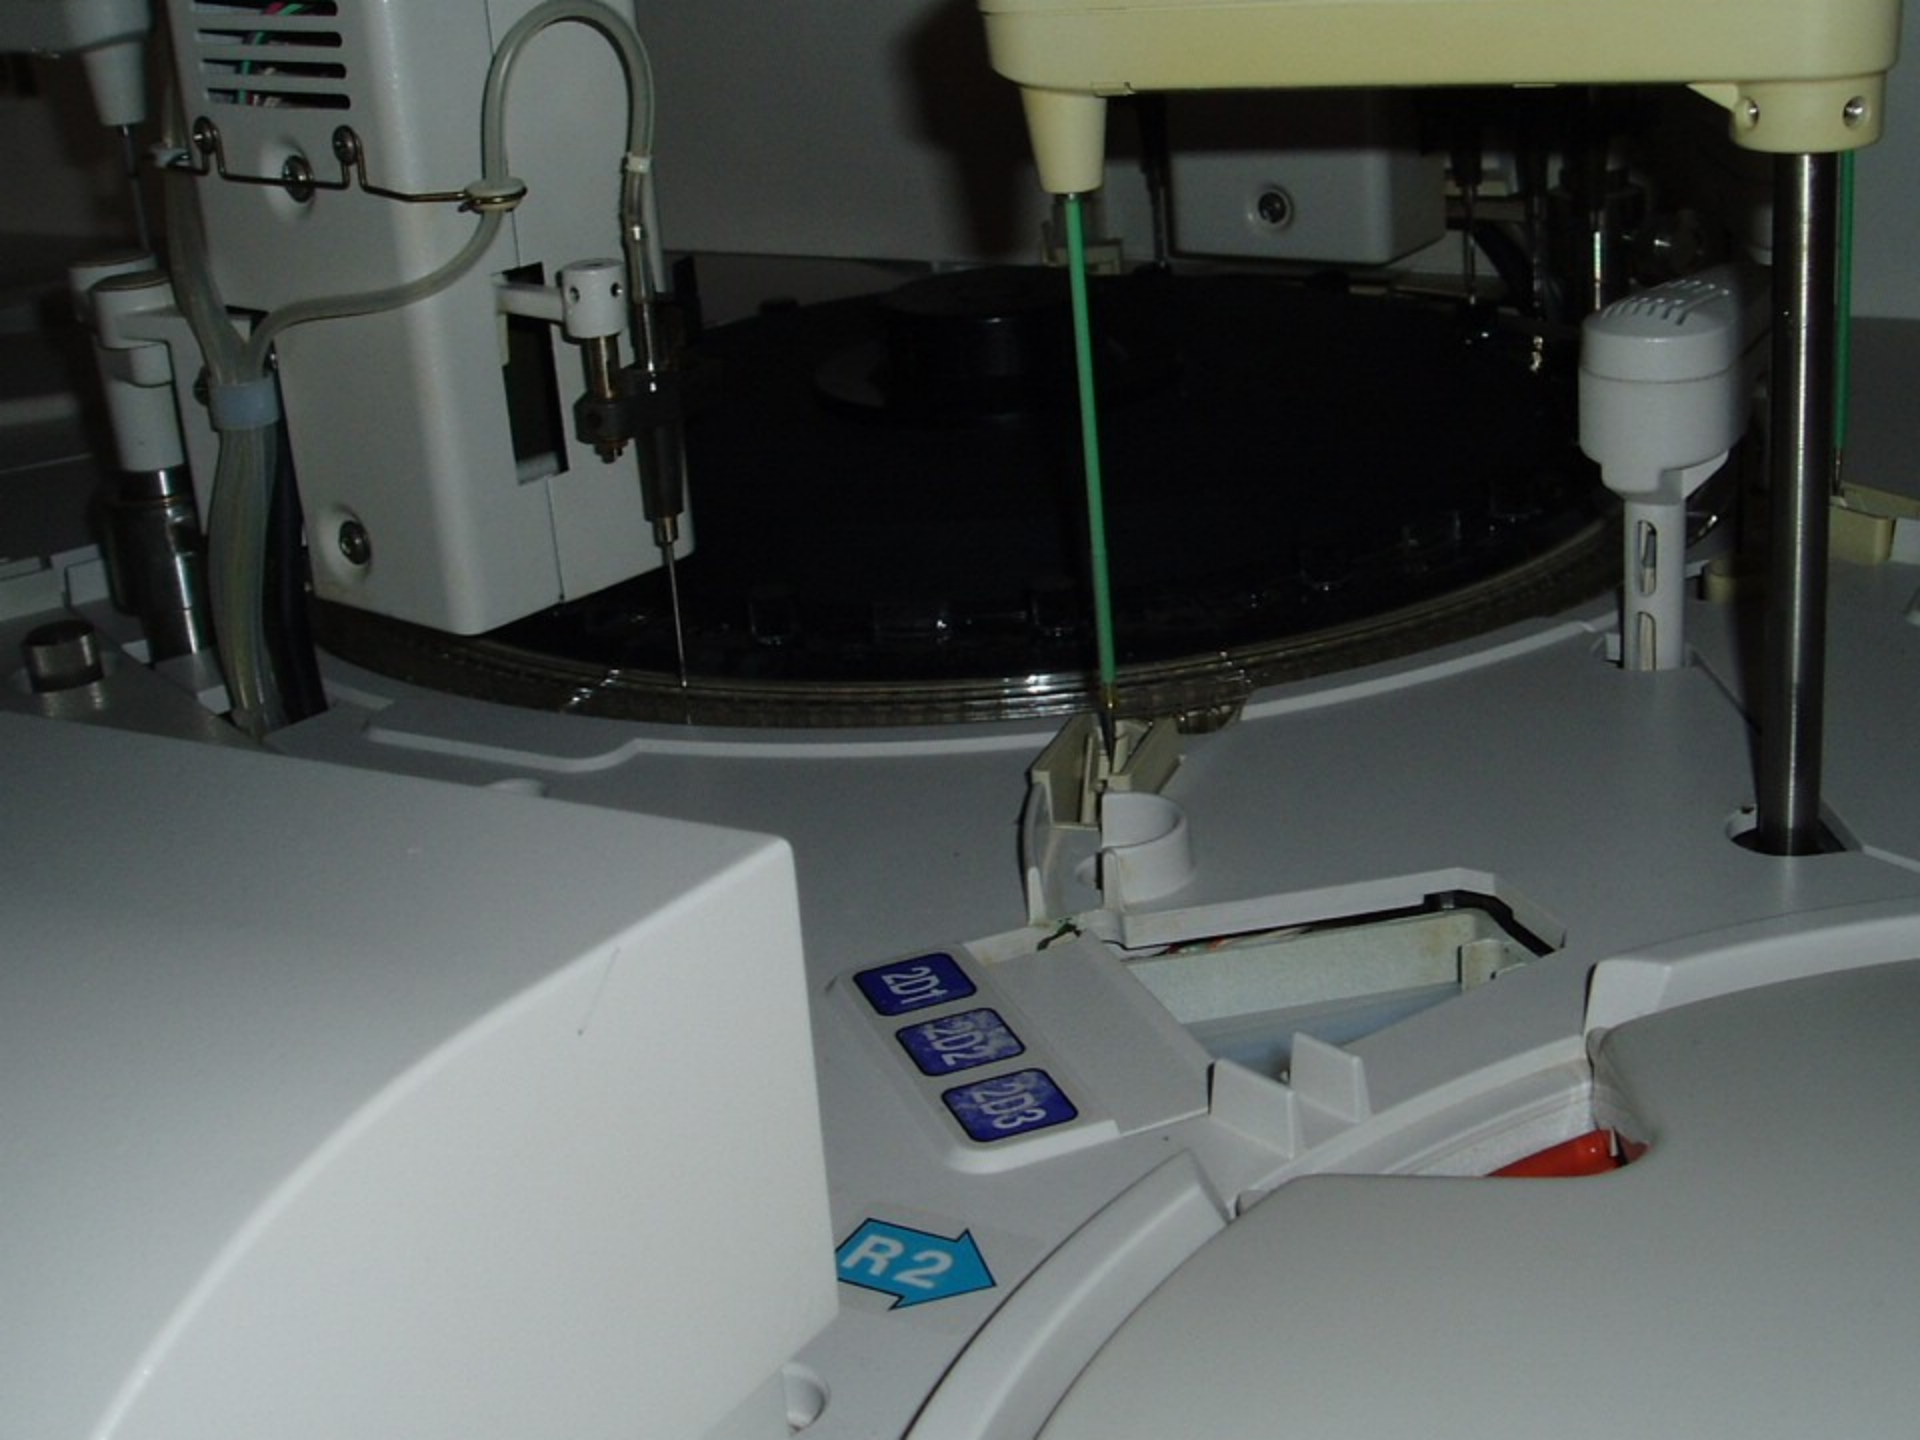

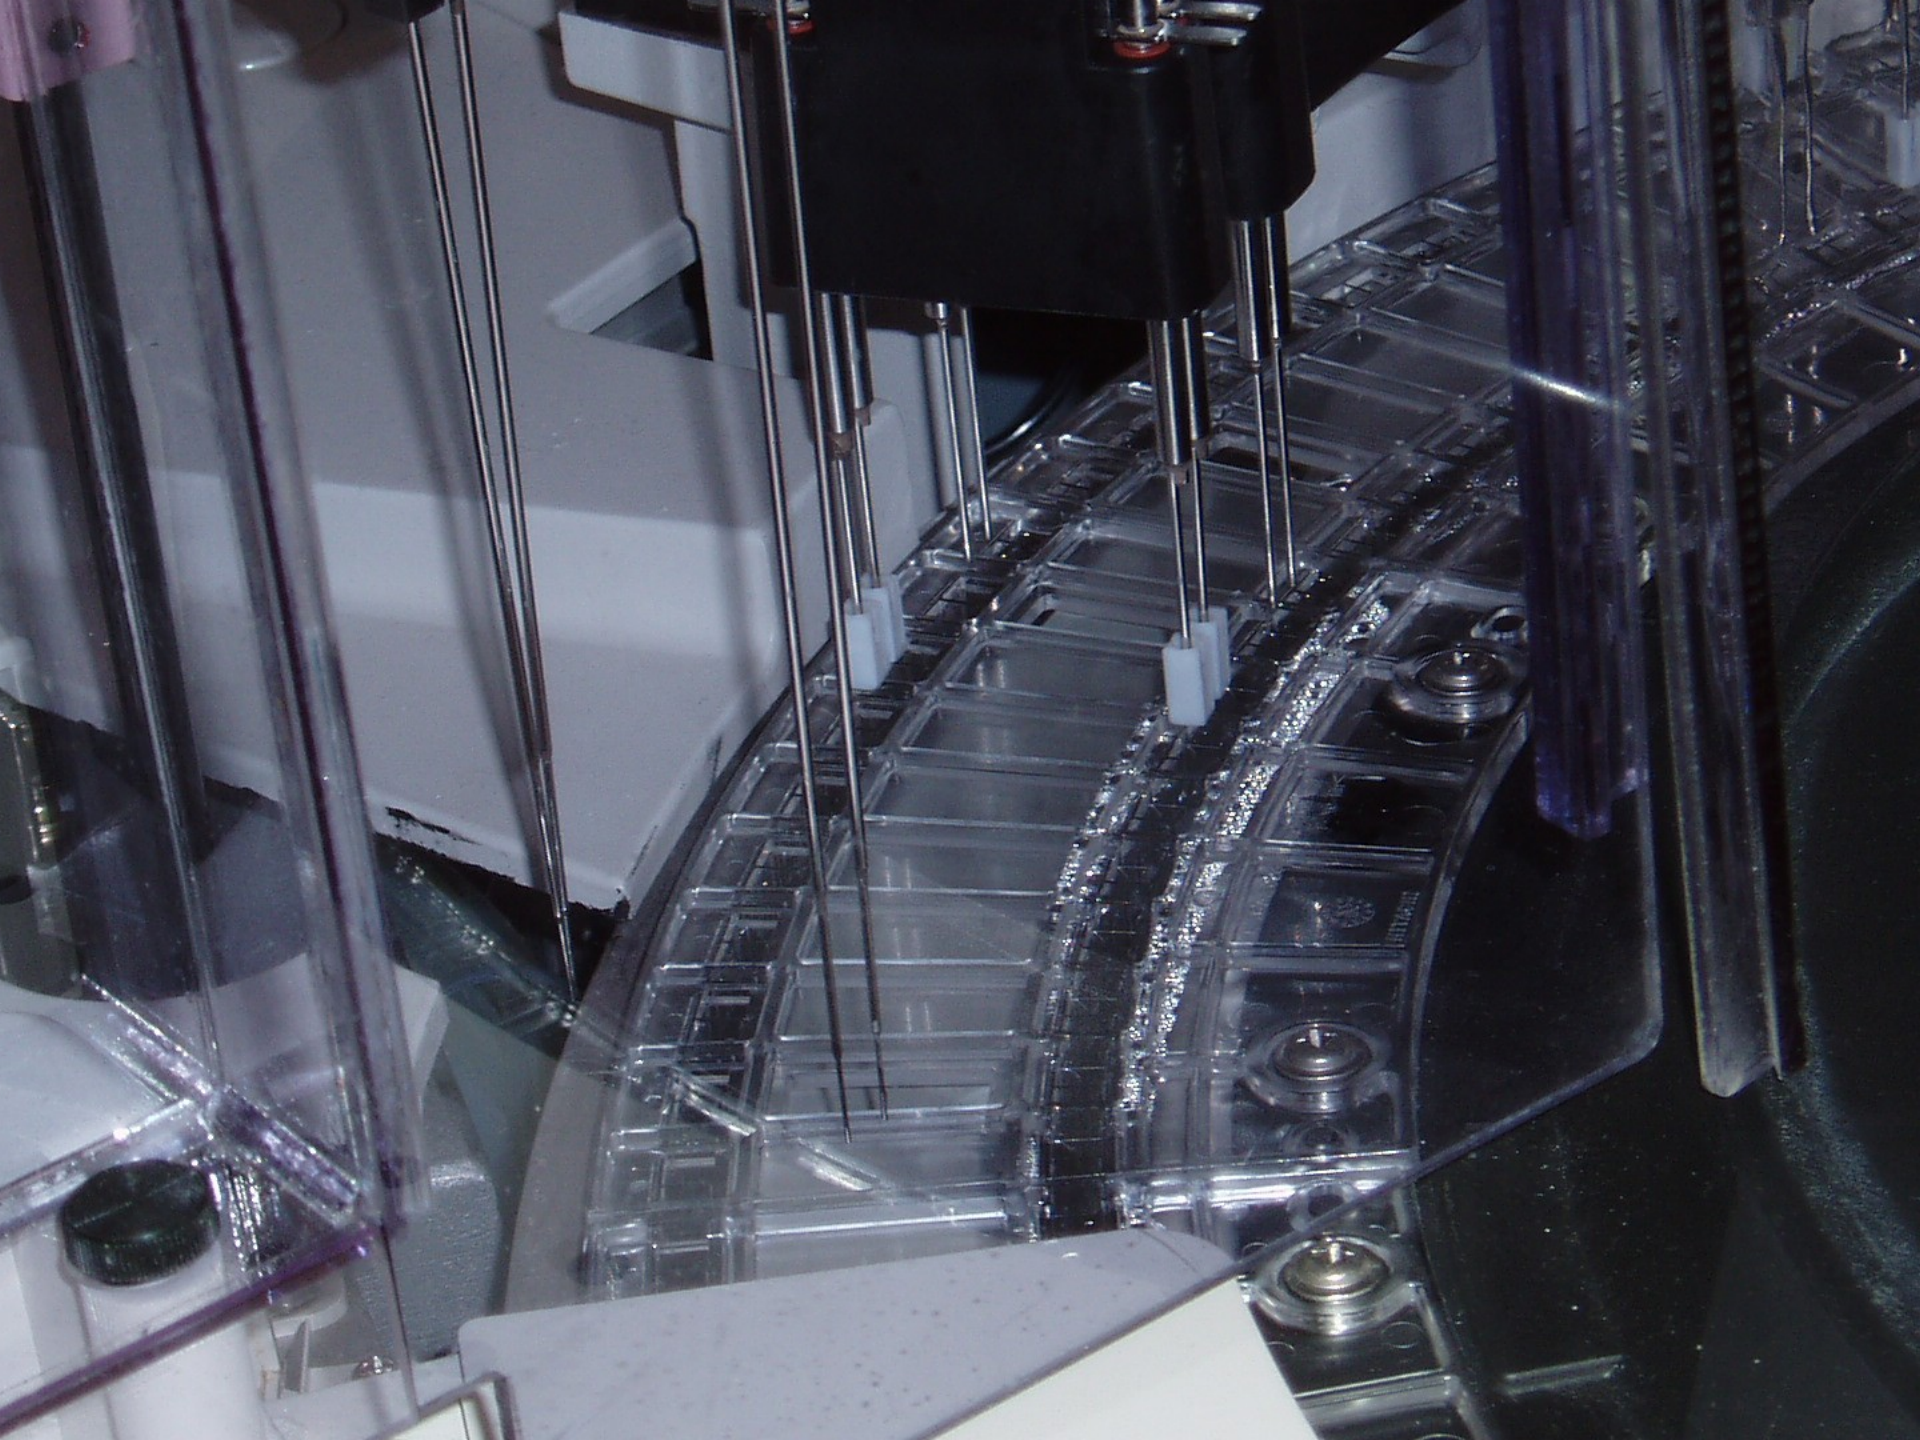



Cell Wash Solution I / NaOH-I

Roche/Hitachi
11551540 316

Cont. 1800 ml

IVD CE 15 - 25°C

LOT 653 870-01 2005 - 12

For USA
Cont. Contents of bid
NaOH 3.7%
Lot Batch code
Use by
Store at
Manufacturer
For in vitro
diagnostic use




Roche Diagnostics GmbH
D-68298 Mannheim
Distributors in USA:
Roche Diagnostics Corporation,
Indenassett, NJ, USA
Made in Germany



COBAS I

Roche
COBAS MIRA



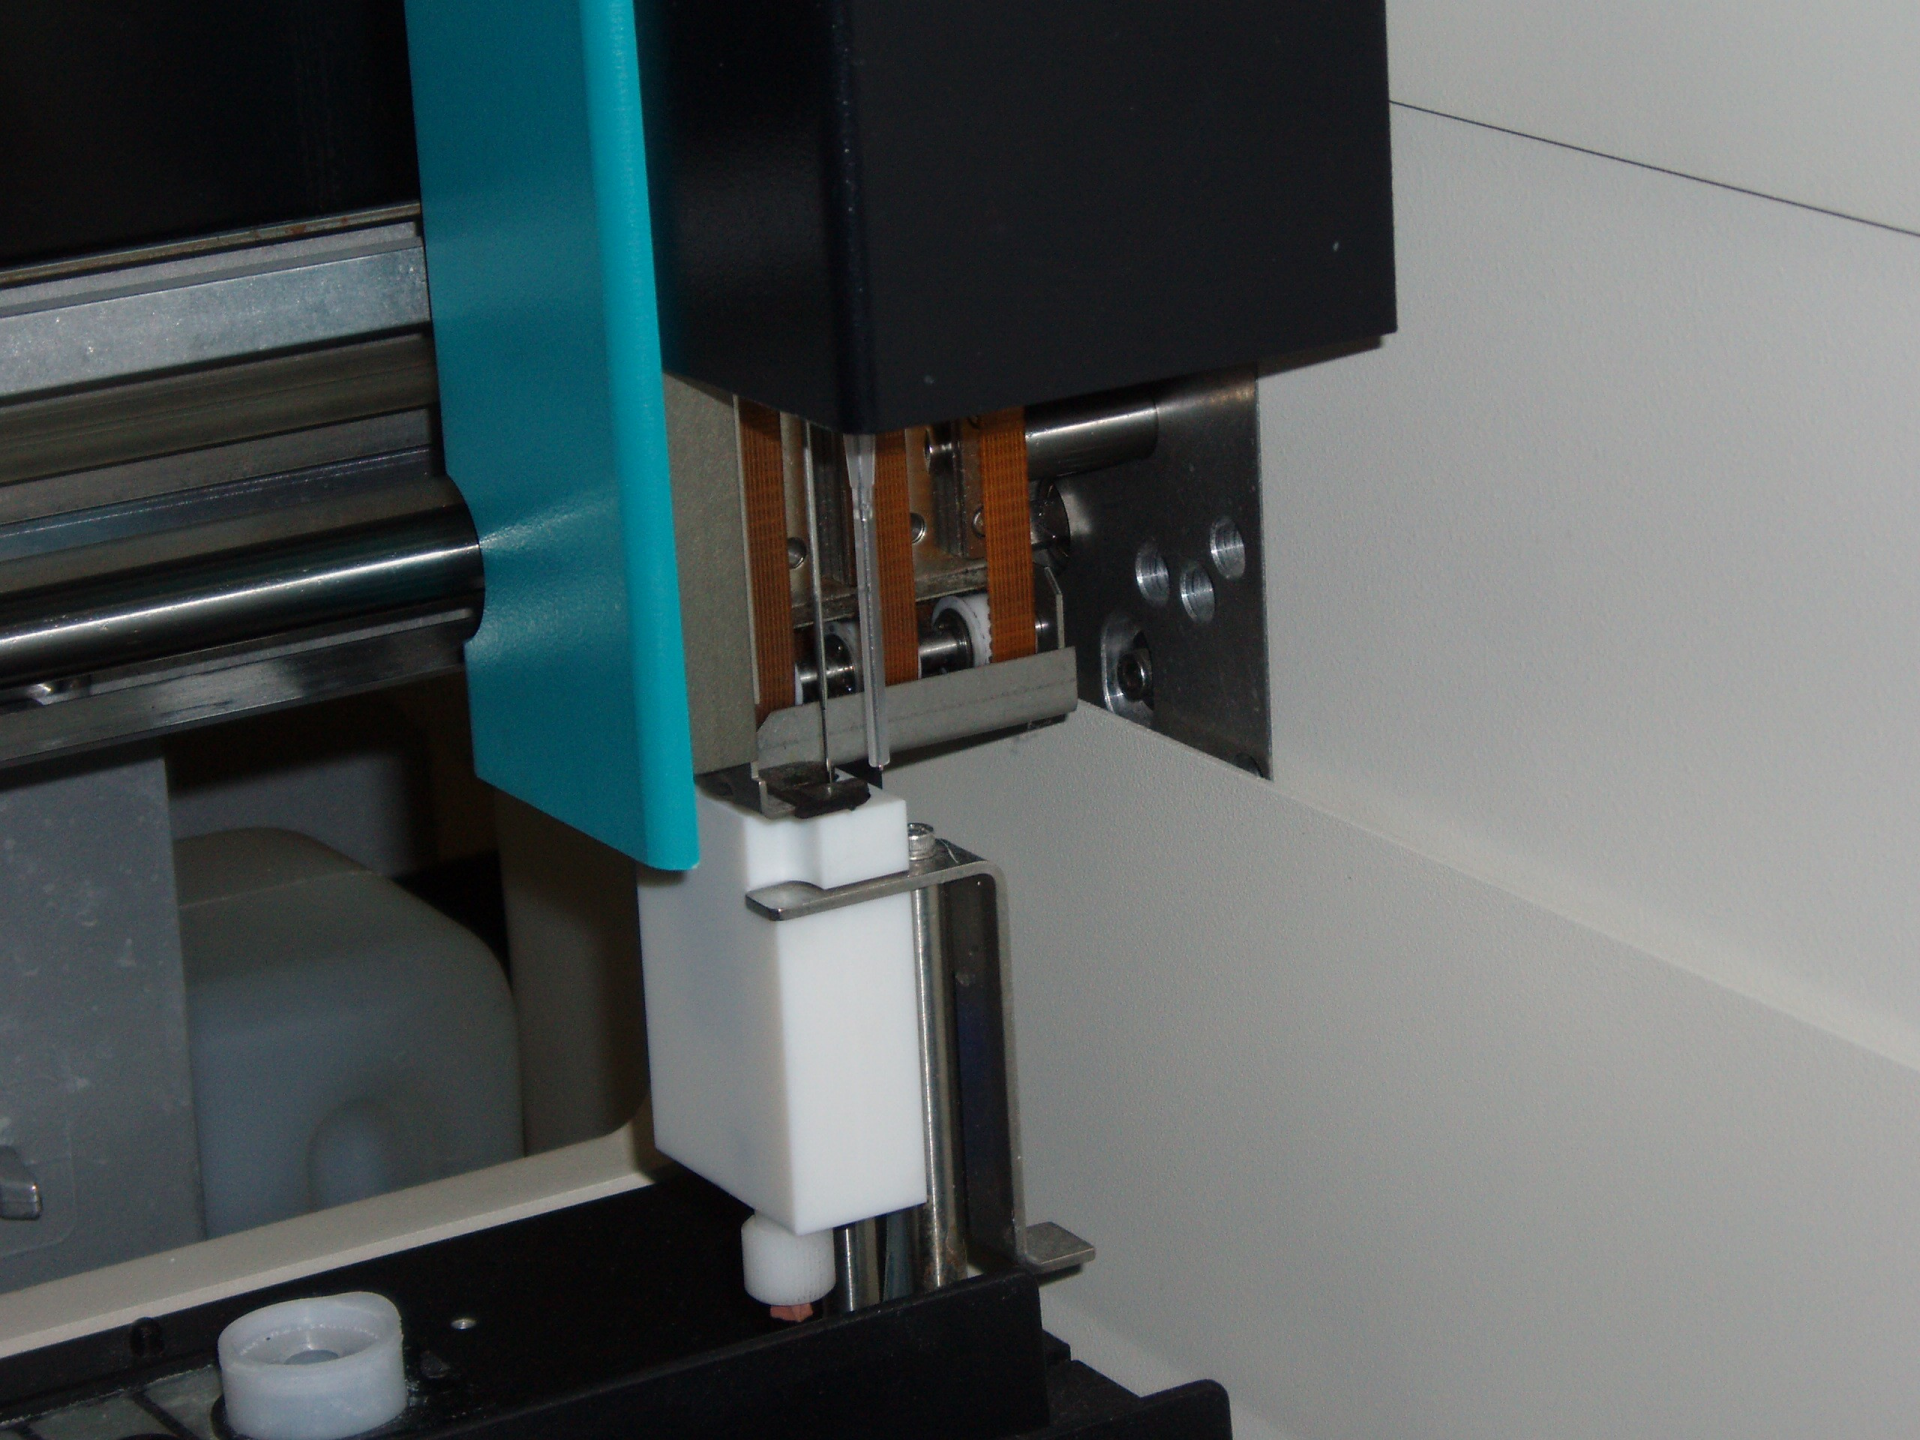





REAGENT 5_s
7
COBAS

REAGENT 5_s
6
COBAS

SAMPLE 30
1
COBAS

C3

C4

A1AT

DAPT

DIL.

ORONA

- | | |
|----|----|
| 1 | 16 |
| 2 | 17 |
| 3 | 18 |
| 4 | 19 |
| 5 | 20 |
| 6 | 21 |
| 7 | 22 |
| 8 | 23 |
| 9 | 24 |
| 10 | 25 |
| 11 | 26 |
| 12 | 27 |
| 13 | 28 |
| 14 | 29 |
| 15 | 30 |

