

# Automatické biochemické analyzátory



Automatic  
Analyzer V.E. 1141-0

HITACHI







AK22  
AK21

1D1 1D2 1D3

R1

Väljnings kodsrad  
CB R1 R2  
MG R1  
KREA R1  
CA R1

A CAUTION  
Always wear safety glasses when using this instrument.

D EF IS

Do not attempt to open the instrument when the rotor is in motion. The rotor is very heavy and can cause injury if it falls. Always use the rotor handle to move the rotor.


WARNING  
Do not attempt to open the instrument when the rotor is in motion. The rotor is very heavy and can cause injury if it falls. Always use the rotor handle to move the rotor.

1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20 21 22 23 24 25 26 27 28 29 30 31 32 33 34 35 36 37 38 39 40 41 42 43 44 45 46 47 48 49 50 51 52 53 54 55 56 57 58 59 60 61 62 63 64 65 66 67 68 69 70 71 72 73 74 75 76 77 78 79 80 81 82 83 84 85 86 87 88 89 90 91 92 93 94 95 96 97 98 99 100


1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20 21 22 23 24 25 26 27 28 29 30 31 32 33 34 35 36 37 38 39 40 41 42 43 44 45 46 47 48 49 50 51 52 53 54 55 56 57 58 59 60 61 62 63 64 65 66 67 68 69 70 71 72 73 74 75 76 77 78 79 80 81 82 83 84 85 86 87 88 89 90 91 92 93 94 95 96 97 98 99 100

1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20 21 22 23 24 25 26 27 28 29 30 31 32 33 34 35 36 37 38 39 40 41 42 43 44 45 46 47 48 49 50 51 52 53 54 55 56 57 58 59 60 61 62 63 64 65 66 67 68 69 70 71 72 73 74 75 76 77 78 79 80 81 82 83 84 85 86 87 88 89 90 91 92 93 94 95 96 97 98 99 100



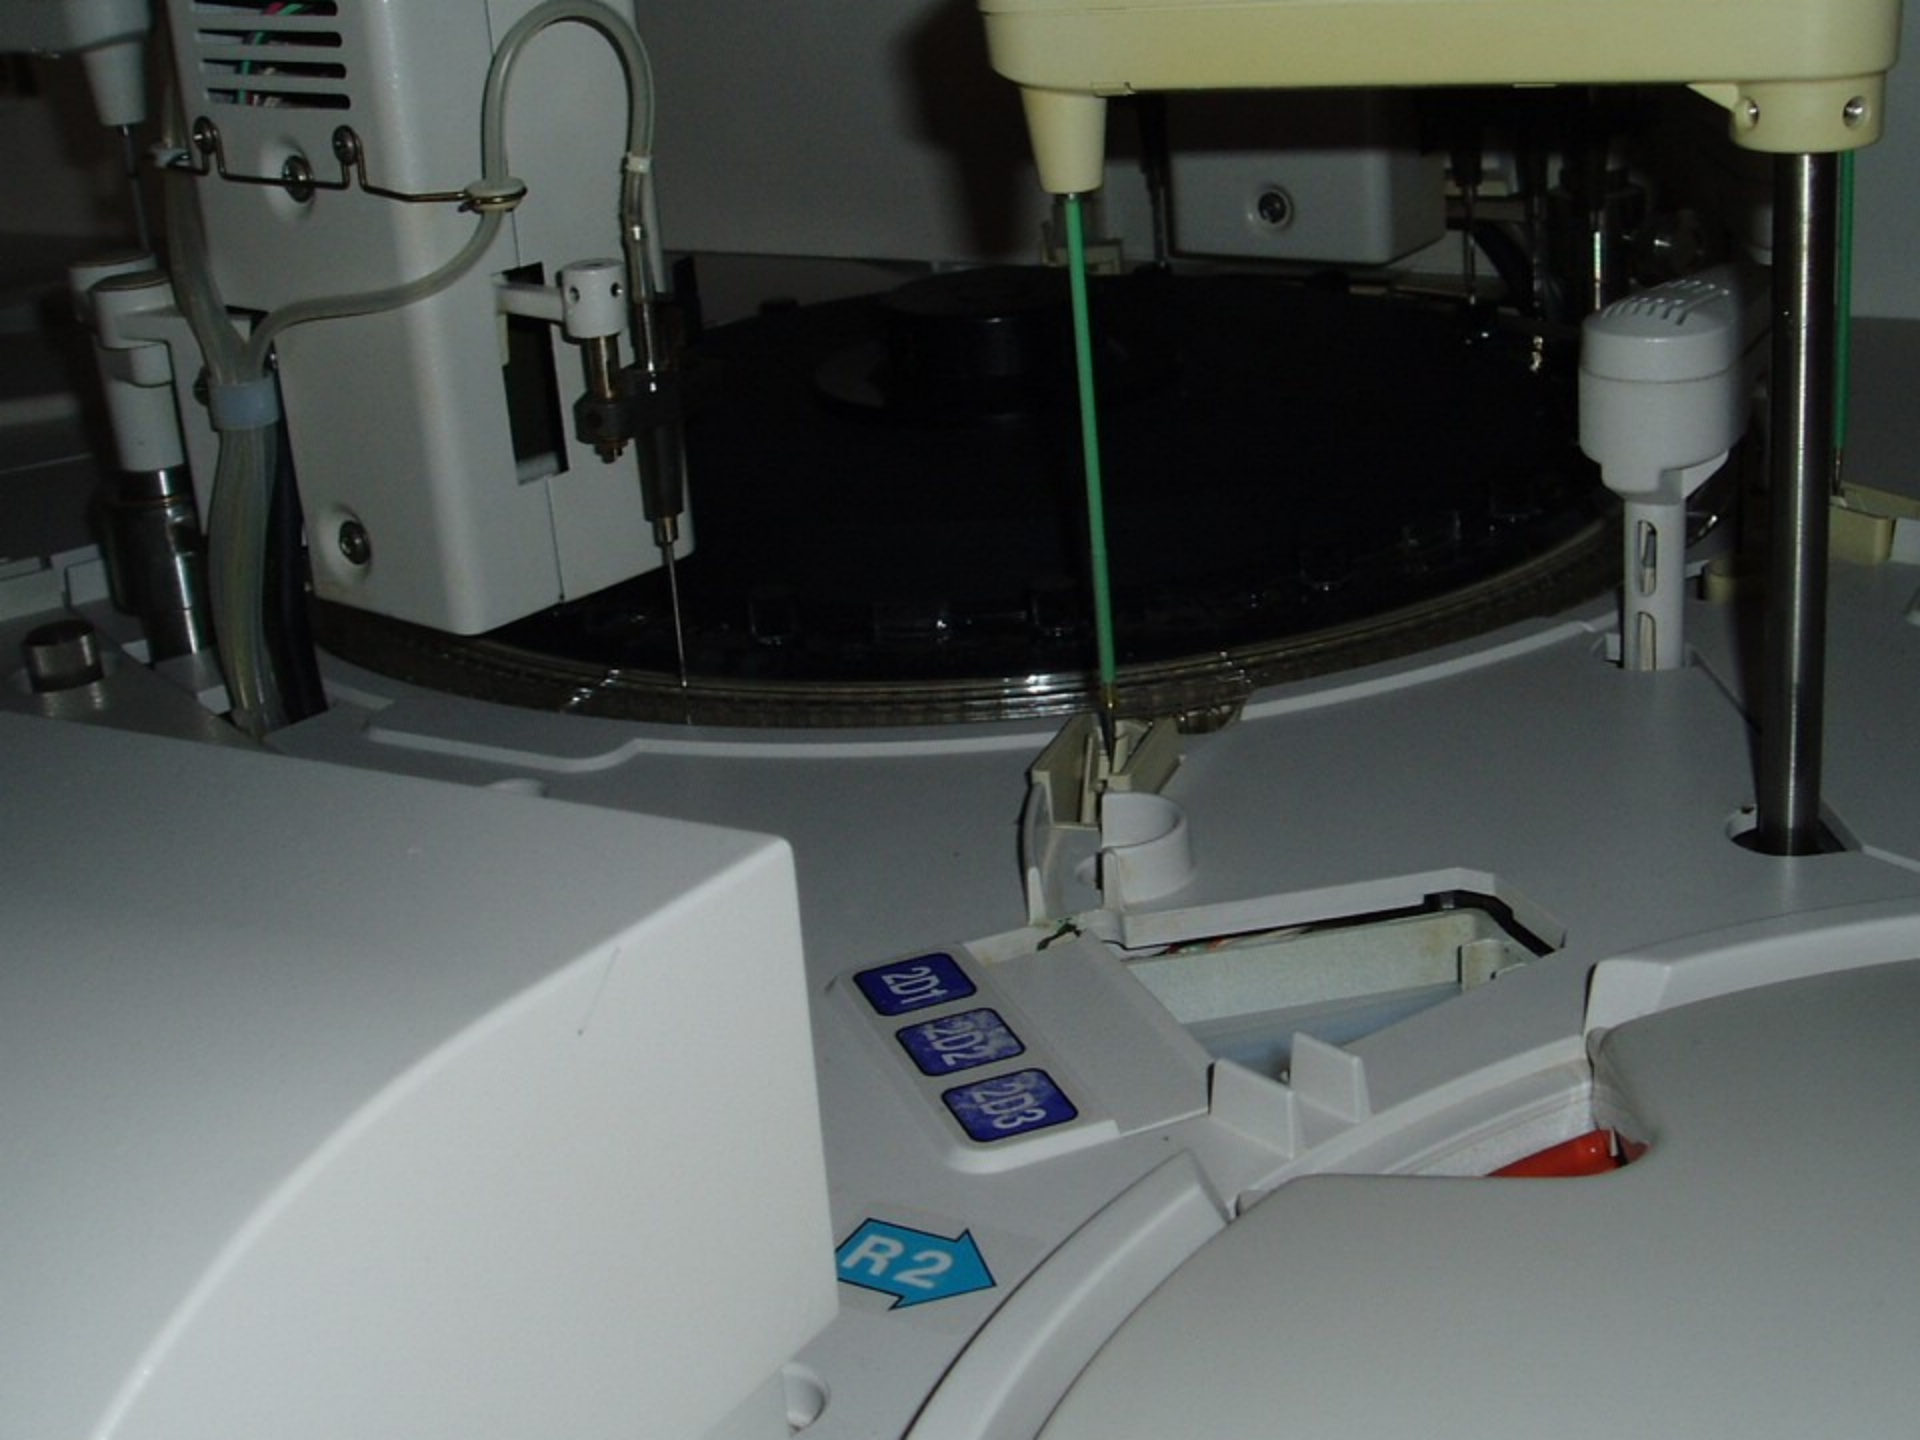



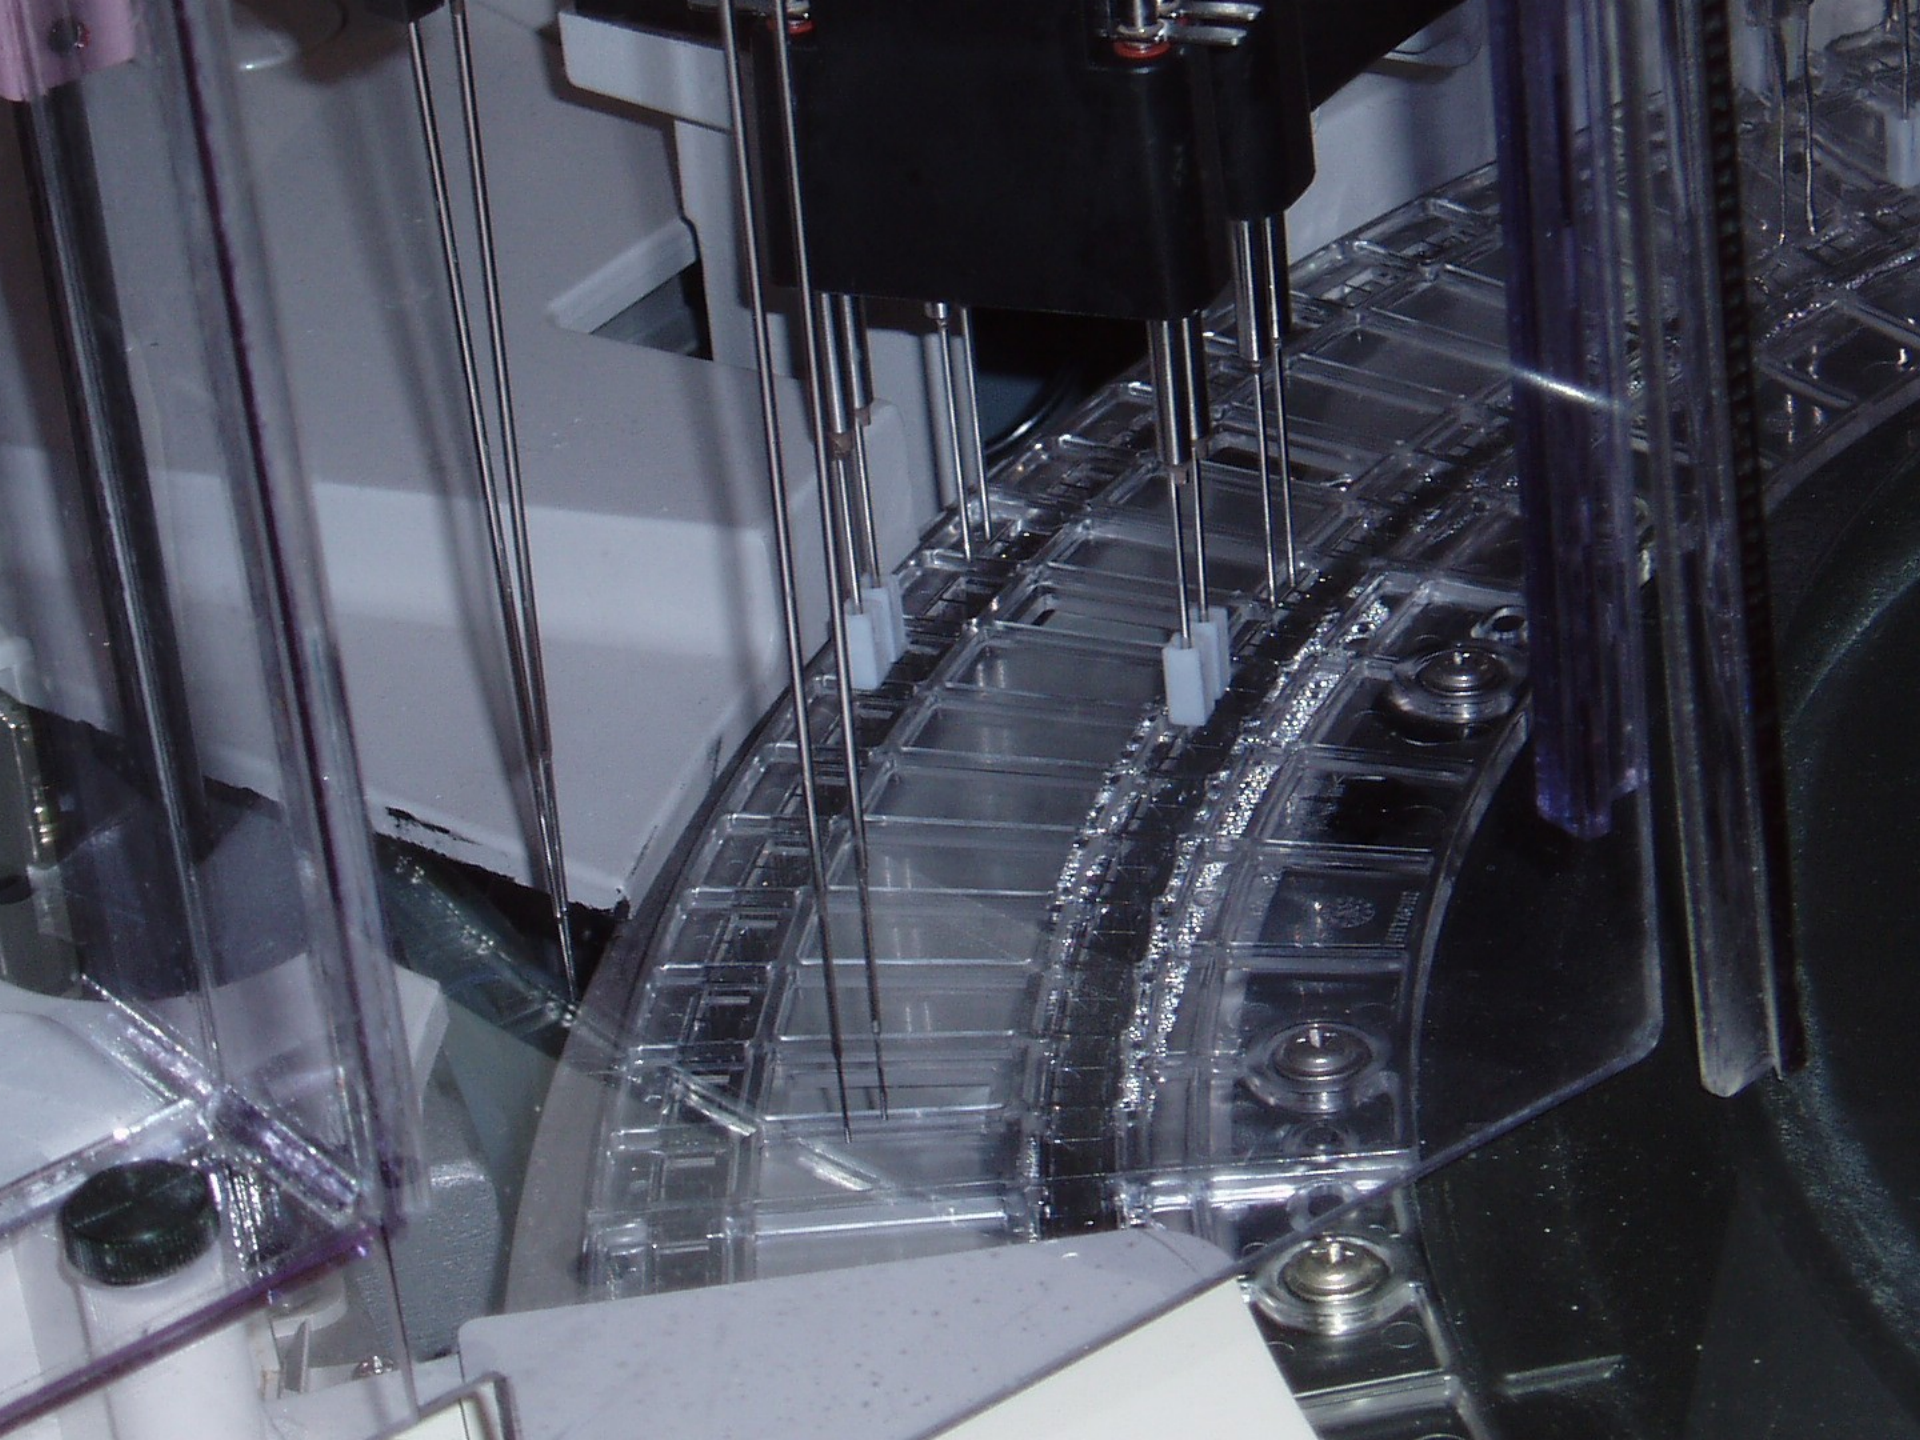


















COBAS I

Roche  
**COBAS** MIRA





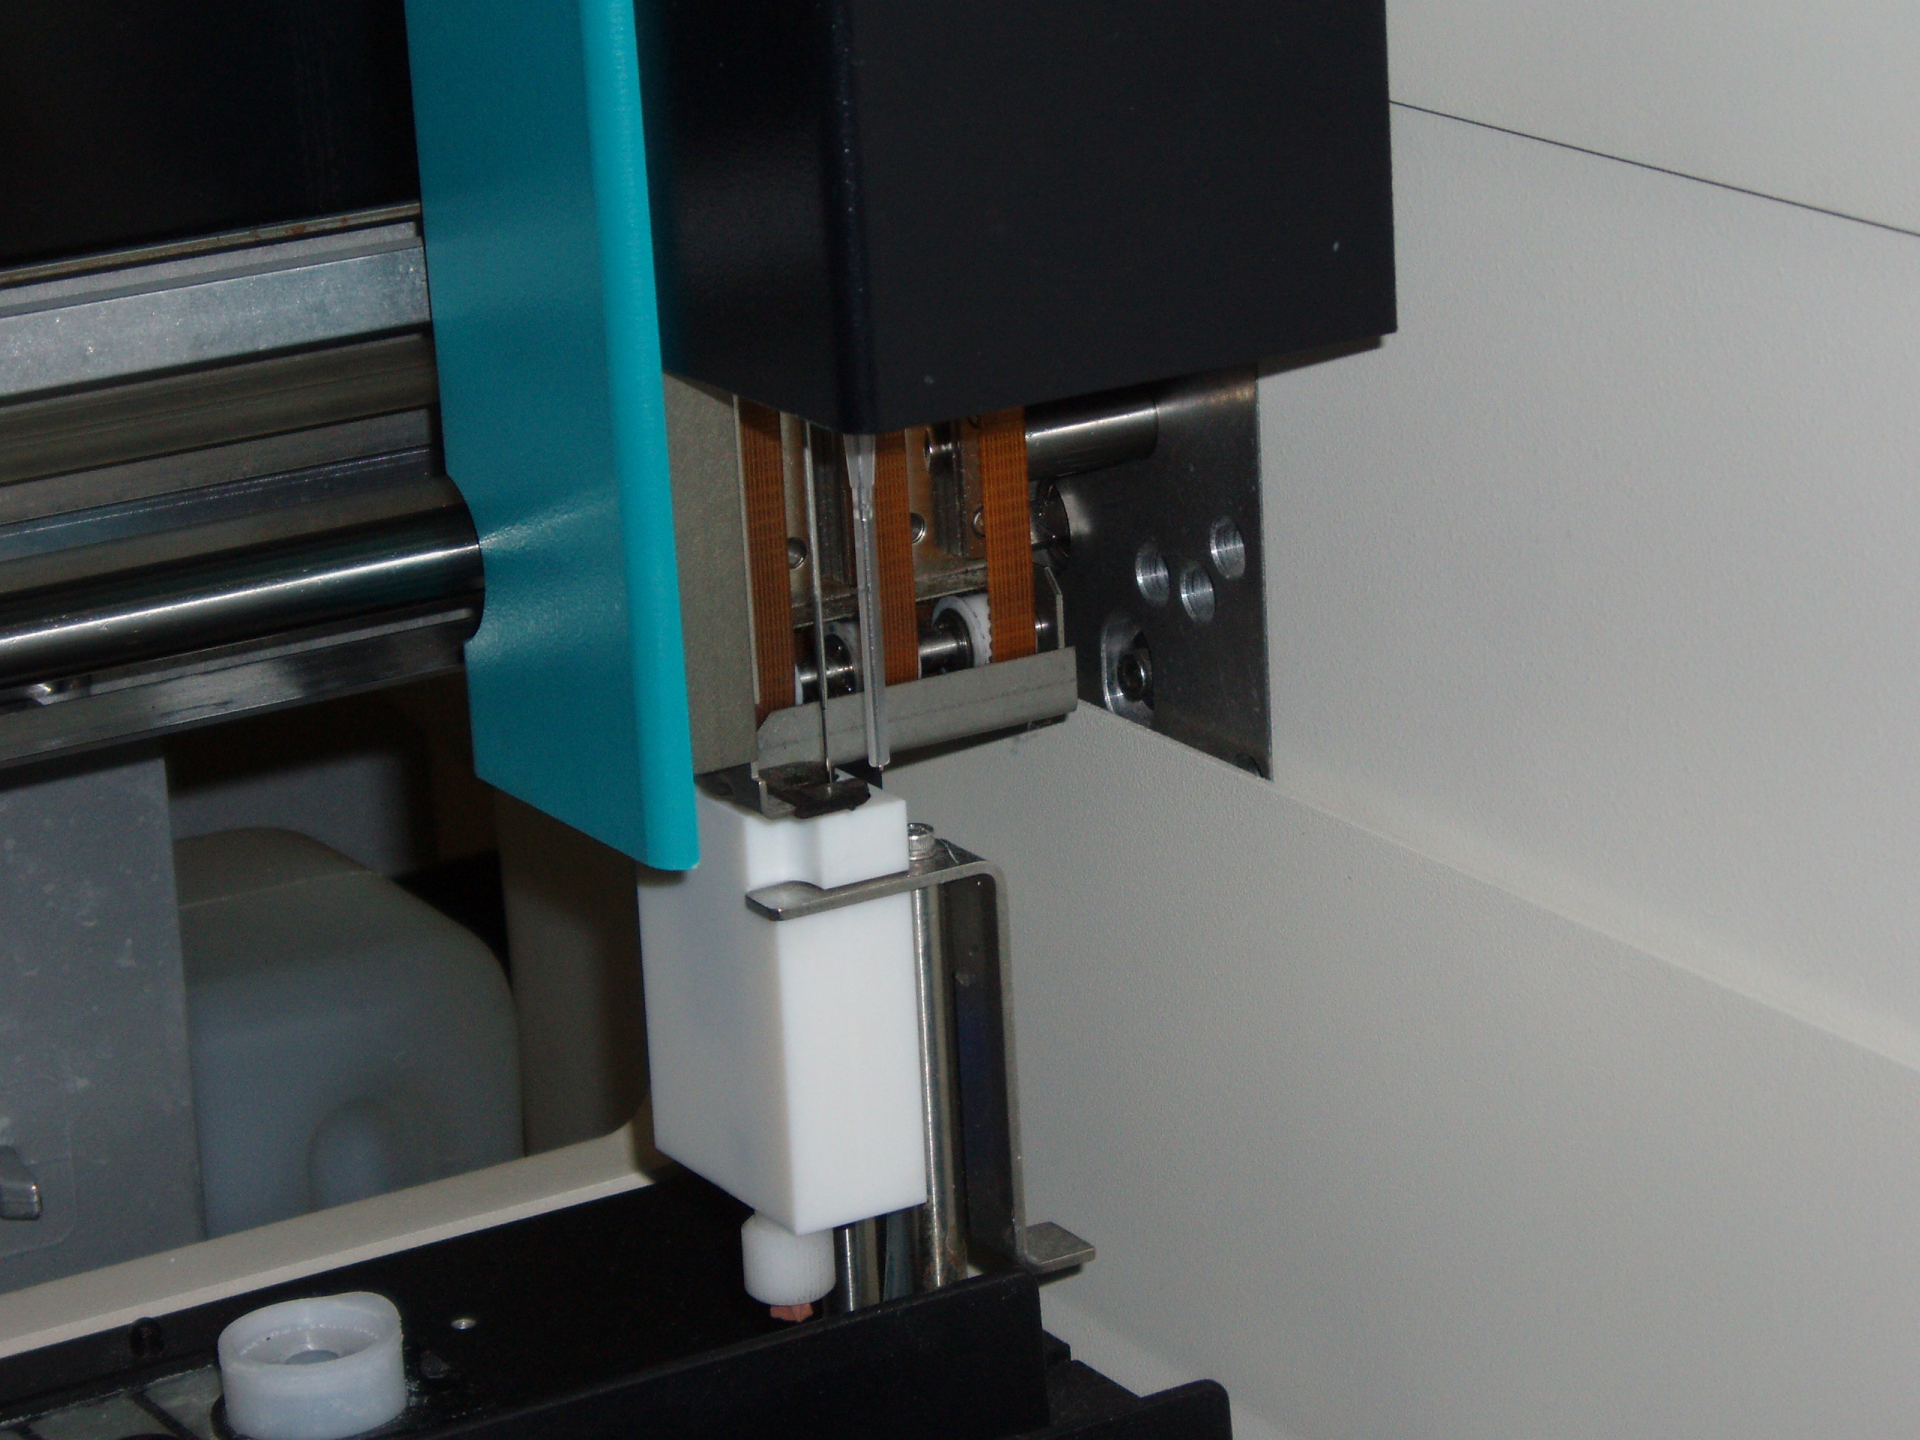









**REAGENT 5<sub>s</sub>**  
**7**  
COBAS

**REAGENT 5<sub>s</sub>**  
**6**  
COBAS

**SAMPLE 30**  
**1**  
COBAS

CL

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8

C3

C4

A1AT

AAPT

ORONA

DIL.

DOX-S

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17
- 18
- 19
- 20
- 21
- 22
- 23
- 24
- 25
- 26
- 27
- 28
- 29
- 30



