




INTRODUCTION TO HISTOLOGICAL TECHNIQUES AND
SAMPLE PREPARATION FOR LIGHT AND ELECTRON
MICROSCOPY

DHE MF MU, 2016

Histology

- Resolution of naked eye – 0,1 mm
- Resolution of light microscopy – 0.5 μm (usually)
- Resolution of electron microscopy – 0,1 nm



Tissue processing for the light microscopy (LM)

(making of permanent preparations – slides)

- **SAMPLING** (obtaining of material – cells, tissue pieces)
- **FIXATION** of samples (tissue blocks)
- **RINSING** (washing) of samples
- **EMBEDDING** of samples - embedded blocks
- **CUTTING** of blocks - sections
- **AFFIXING** of sections
- **STAINING** of sections
- **MOUNTING** of sections

SAMPLING

- A small piece of organ (tissue) is sampled and quickly put into the fixative medium.
- Biopsy during surgical dissection of organs in living organism
 - = excision
 - = puncture (liver or kidney parenchyma, bone marrow)
 - = curettage (uterine endometrium, adenoid vegetation)
- Necropsy from dead individual (sections); in experiments laboratory animals are used and tissue have to be sampled as soon as possible after the break of blood circulation
- The specimens shouldn't be more than **5 – 10 mm³** thick and fixation should follow immediately.

FIXATION

- Definition: denaturation and stabilization of cell proteins with minimum artifacts)
- The reason of fixation: freshly removed tissues are chemically unstable – dry, shrink, undergo hypoxia, autolysis and bacteriological changes
- To stop or prevent these changes and preserve the structure tissue samples have to be fixed. During the fixation, all tissue proteins are converted into inactive denaturated (stable) form.
- 3 main requirements on fixatives:
 - good preservation of structure
 - quick penetration into tissue block
 - no negative effects on tissue staining

- Fixatives: solutions of various chemicals
 - organic fixatives – ALDEHYDES – formaldehyde (*most frequently used for LM*)
 - glutaraldehyde (*used for EM*)
 - ALCOHOLS – 96 – 100 % (absolute) ethylalcohol
 - ORGANIC ACIDS – glacial acetic acid, picric acid, trichloroacetic acid
 - inorganic fixatives – INORGANIC ACIDS – chromic acid, osmium tetroxide (OsO₄)
 - SALTS OF HEAVY METALS – mercuric chloride HgCl₂
 - compound fixatives – mixtures (two or more chemical components to offset undesirable effects of individual (simple) fixatives.
 - FLEMMING's fluid – with OsO₄
 - ZENKER's and HELLY's fluid, SUSA fluid – with HgCl₂
 - BOUIN's fluid – with picric acid
 - CARNOY's fluid – with alcohol

Performance: fixatives are carried out at room temperature, the duration varies between **12 – 24 hours**, specimen must be covered by 20 – 50 times fixative volume:

Ratio of tissue block volume to fixative volume 1 cm³ : 20 – 50 cm³

RINSING and EMBEDDING

- All samples should be washed to remove the excess of fixative; the choice of rinsing medium is determined by type of fixative: running tap-water or 70-80% ethanol
- Relevance of embedding: tissues and organs are brittle and unequal in density, they must be hardened before cutting

Embedding media

- water soluble – gelatine, celodal, water soluble waxes
- anhydrous – paraffin, celoidin

EMBEDDING into PARAFFIN

- dehydration – to remove water from fixed samples by ascending series of ethanol is used (50%, 70%, 90%, 96%. each step - 2 – 6 hours
- clearing – the ethanol must be replaced with organic solvantant that dissolves paraffin – benzene or xylene
- infiltration – melted paraffin wax (56°C) is used; 3 x 6 hours.
- casting (blocking out) – moulds (plastic, paper or metal chambers) are used for embedding.
 - The moulds are filled with melted paraffin, tissue samples are then placed inside and immediately immersed in cold water to cool paraffin quickly down.
 - These paraffin blocks are ready for trimming




Leica TP 1020

Automated device for tissue dehydration




Paper chambers

- metal




CUTTING


- Microtome – a machine with automatic regulation of section thickness: 5 – 10 μm is optimum.



sliding microtome – block is fixed in holder, knife or razor moves horizontally



rotary microtome – knife is fixed, block holder moves vertically



Sliding microtome




Rotary microtome

Freezing microtome (**cryostat**)
= rotary microtome housed in freezing box
(- 60° C)


Cutting of frozen tissue without embedding






sampling

1




fixation

2




fixation

3



cutting

4




cutting

5




section affixing



6



section affixing

7





AFFIXING


- Mixture of glycerin and egg albumin or gelatin
- Section are transferred from microtome razor or knife on the level of warm water (45° C), where they are stretched; then they are put on slides coated with adhesive mixture; excess of water is drained and slides are put in incubator (thermostat, 37° C) over night to affixing of sections.



Stretching of sections on warm water



Stretching on a warm plate



STAINING

- Different cell or tissue structures are not apparent without staining.
- Cellular structures exhibit different affinity to staining dyes

alkaline dyes (basic or nuclear) – react with anionic groups of cell and tissue components

basophilia – basophilic structures in the cell

acid dyes (cytoplasmic) – react with cationic groups



acidophilia – acidophilic structures in the cell

neutrophilia – no reaction


Staining methods:

routine – HE, AZAN

(demonstrate all components of tissue)




HE – the most frequent used method



special


visualizes only special structures



*Lipid droplets
detected by oil red*

impregnation

by silver salt for detection
of nerve or reticular fibers



ROUTINE STAINING with HEMATOXYLINE – EOSIN (HE)


Hematoxyline – basic (nuclear) dye

Eosin – acid (cytoplasmic dye



- Staining procedure:
- paraffin must be removed (dissolved) by xylene
- sections are rehydrated in descending series of ethanol (100% →96% →80%)
- staining with hematoxyline
- differentiation in acid ethanol and water (excess of dye is removed)
- staining with eosin
- rinsing in water (excess of dye is removed)
- dehydration in graded ethanol series (80% →96% →100%)
- clearing in xylene

HEMATOXYLINE – EOSIN (HE)

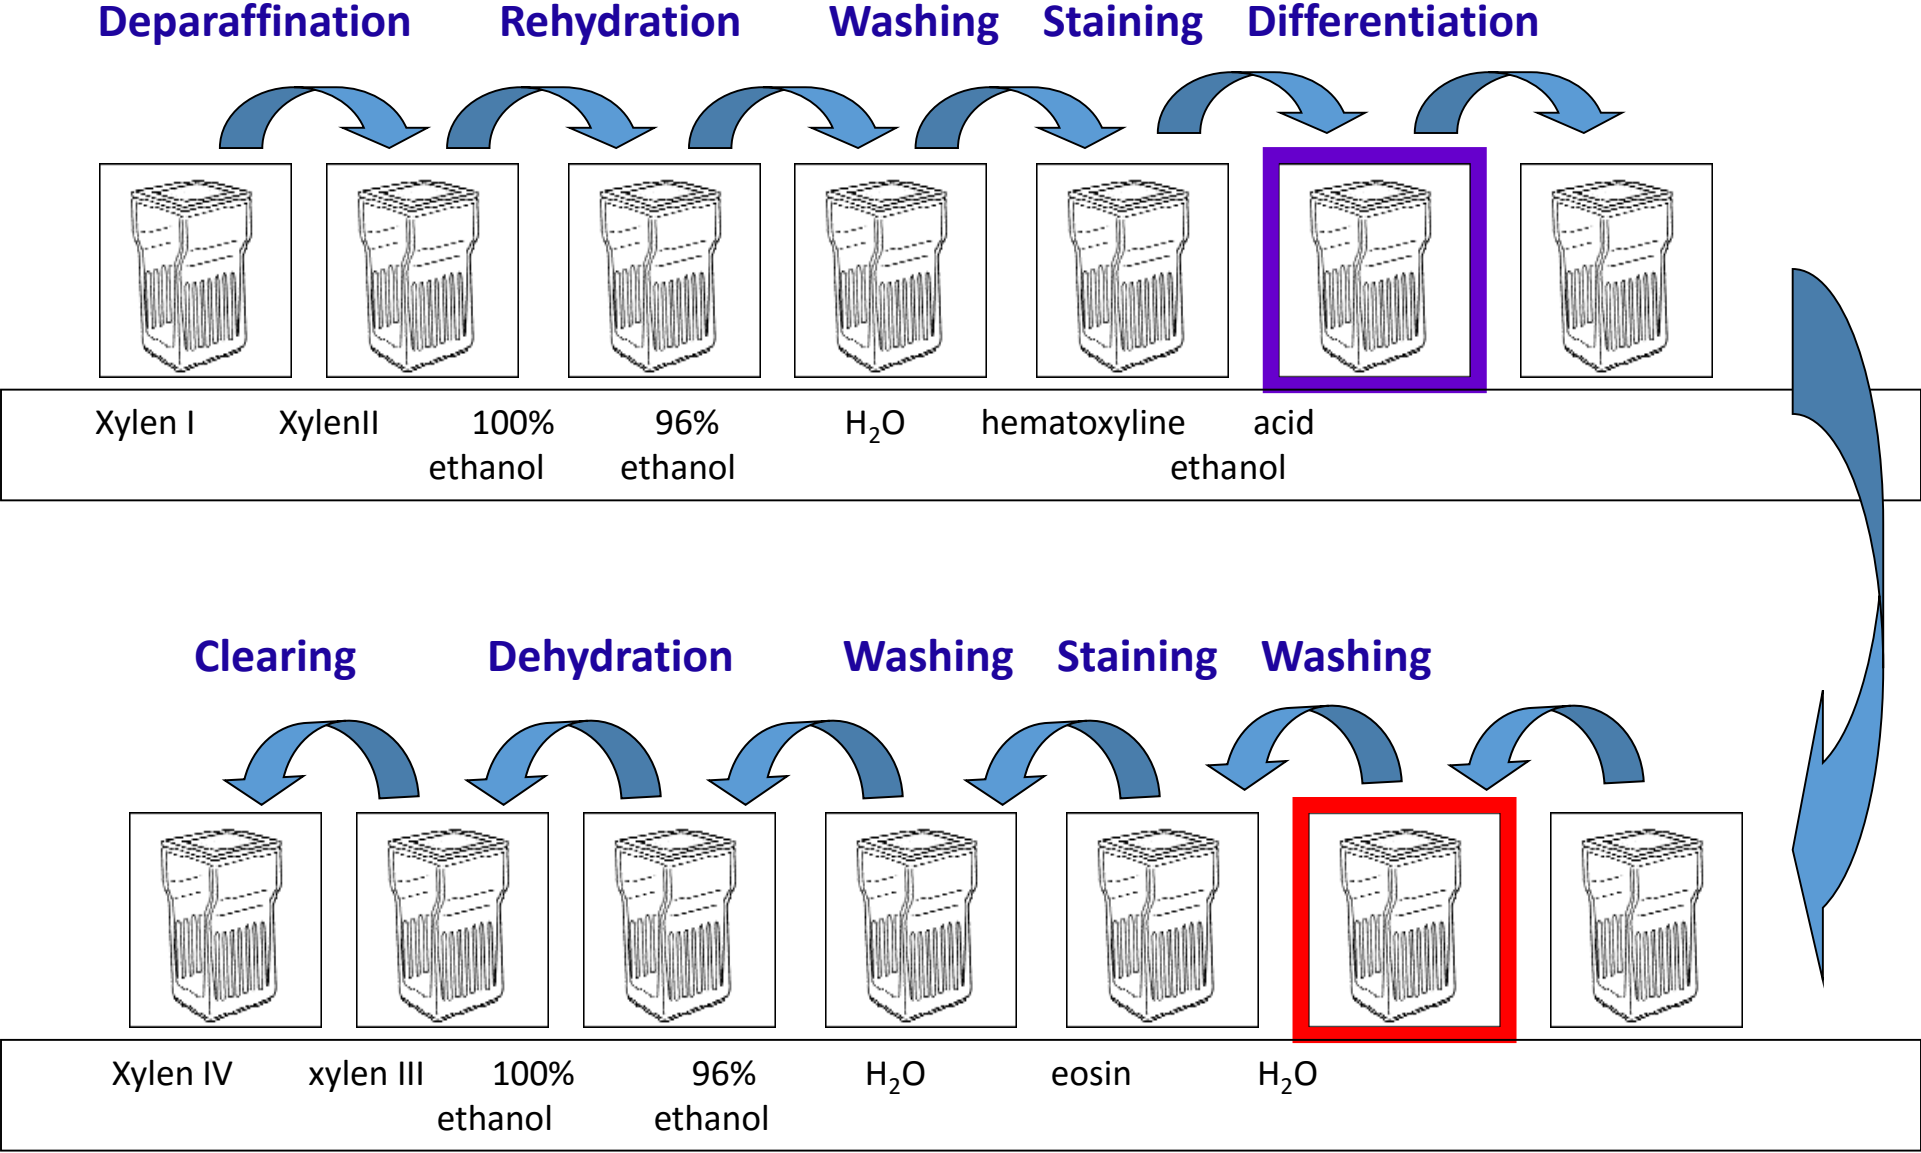

Staining results:

- **HE** = *Hematoxyline – Eosin*
nuclei – bright clear blue or dark violet
cytoplasm and collagen fibers – pink
muscle tissue – red


- **HES** = *Hematoxyline – Eosin – Safron*
connective tissue – yellow

- **AZAN** = *AZocarmin – ANiline blue – orange G*
nuclei – red
erythrocytes – orange
muscle – red
collagen fibers – blue


Staining tools:



cuvette



flask



slides holder
(basket)



Automatic slide stainer





staining set of boxes with media



MOUNTING

- Finally, preparates are closed with coverslip (coverglass) to form a permanent preparate. Small amount of mounting medium must be placed between stained section and the coverslip.




- **Mounting media:** soluble in xylene – **canada balsam**
soluble in water – glycerin-gelatine, arabic gum




Permanent histological slides for study in the light microscope

Hematoxyline and eosin (HE)





Hematoxyline, eosin and saffron (HES)



cartilage

Collagenous fibers
of connective tissue
are yellow after staining
with saffron

Azocarmine and aniline blue (AZAN)




Kidney – collagen connective tissue

Impregnation of tissue with silver




Lien - reticular fibers




Cerebellum – nerve fibers

Iron hematoxyline



Skeletal muscle cells (fibers)

Green trichrome



Histochemistry and Immunohistochemistry

- Relevance:


various chemical compounds detected „in situ“ (proteins, AA, NA, saccharides, lipids, enzymes, pigments, inorganic substances – Fe, Ca, Zn)


Various epitopes detected by immunotechniques

Enzyme conjugated
with secondary Ab -
visualization

Secondary Ab specific
against primary Ab

Primary Ab specific
against epitope of the
particular antigen








Actin (cytoskeleton)




DAPI (nucleus)

Microtubules (cytoskeleton)



Tissue processing for the EM

- pH of all solutions (media) must be buffered on **7.2 – 7.4**
Cacodylate or phosphate buffer is frequently used.
- Absolutely dustfree environment
- Solutions (media) have to be precise (artifacts)



Tissue processing for the EM


- **SAMPLING** – immediately after arresting of blood circulation, tissue block sized no more than **1mm³**
- **FIXATION** – **glutaraldehyde** (binds amine groups) + **OsO₄** (binds lipids) are used as double fixation
- **RINSING** – distilled water
- **DEHYDRATION** - ethanol
- **EMBEDDING** – gelatin capsule or plastic forms are filled with some medium (which can be polymerized from liquid to solid form) and pieces of fixed tissue are placed into this medium. Epoxyd resins (Epon, Durcupan, Araldite) are usually used as in water insoluble media.
- **CUTTING** – ultrathin sections (in ultramictomes)
- **CONTRASTING** ≈ staining

EMBEDDING

gelatin (1) or plastic (2) capsules

capsule holder (3)





embedding plates
(4, 5)






Embedded blocks
prepared for cutting



CUTTING



Grid Types and Mesh Sizes



CUTTING


Ultrathin sections (70 – 100 nm) -
ultramicrotomes.

Glass or diamond (b) knives with water
reservoir are used

Sections slide flow on water in small
container attached to the knife

Supporting grids







Ultramicrotom knives:


glass

diamond



CONTRASTING (=STAINING)

- principle of differentiation of structures – different dispersion of beam of electrons depending on atomic weight of elements.
„electron dyes“ are thus mixtures of heavy metals: uranylacetate or lead citrate



Differences between LM and EM

	LM	EM
Sampling	< 1 cm ³ minutes	< 1 mm ³ seconds
Fixation	formaldehyde 12 – 24 hours	glutaraldehyde 1 – 3 hours
Embedding	paraffin	epoxid resins (Durcupan)
Cutting	microtome	Ultramicrotomes
Thickness of sections	5 – 10 μm	50 – 100 nm
Staining (LM) contrasting (EM)	dyes (hematoxyline – eosin)	heavy metals (uranylacetate, lead citrate)
Mounting (only LM)		---
Result	histological slide (preparate)	photograph of ultrathin section

