



Lectures on Medical Biophysics

Department of Biophysics, Medical Faculty,
Masaryk University in Brno

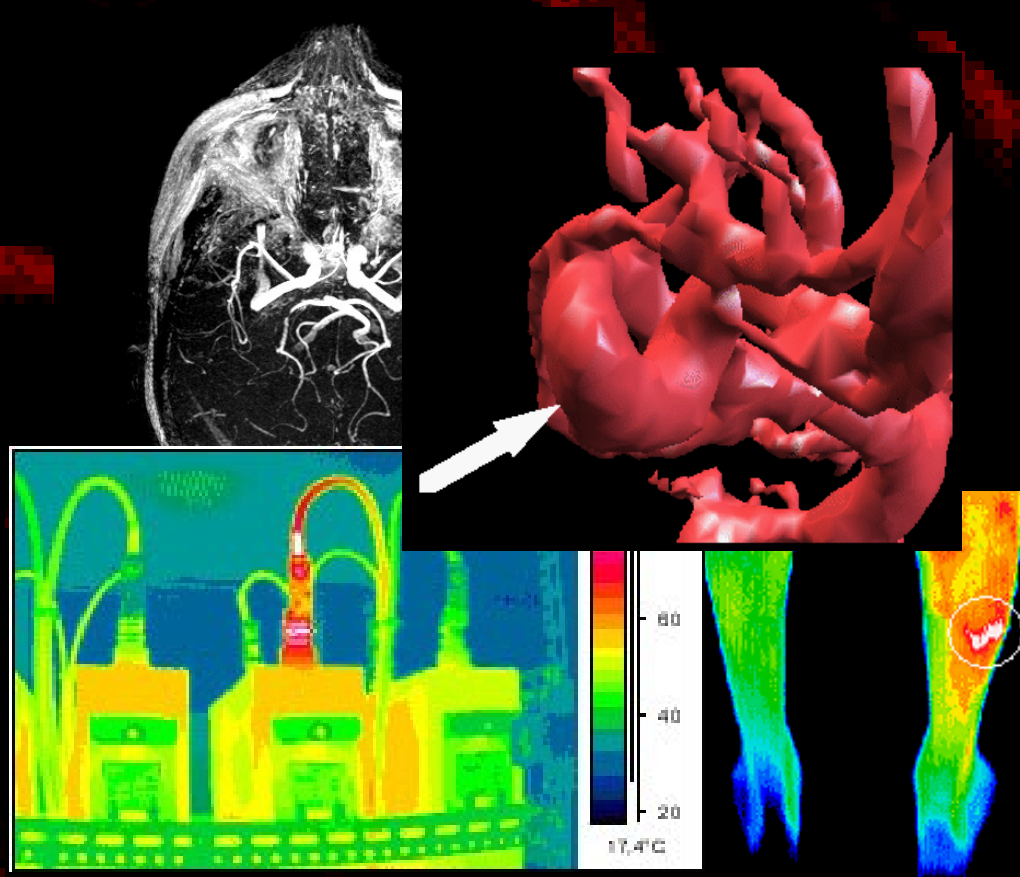

Lectures on Medical Biophysics

Department of Biophysics, Medical Faculty,
Masaryk University in Brno

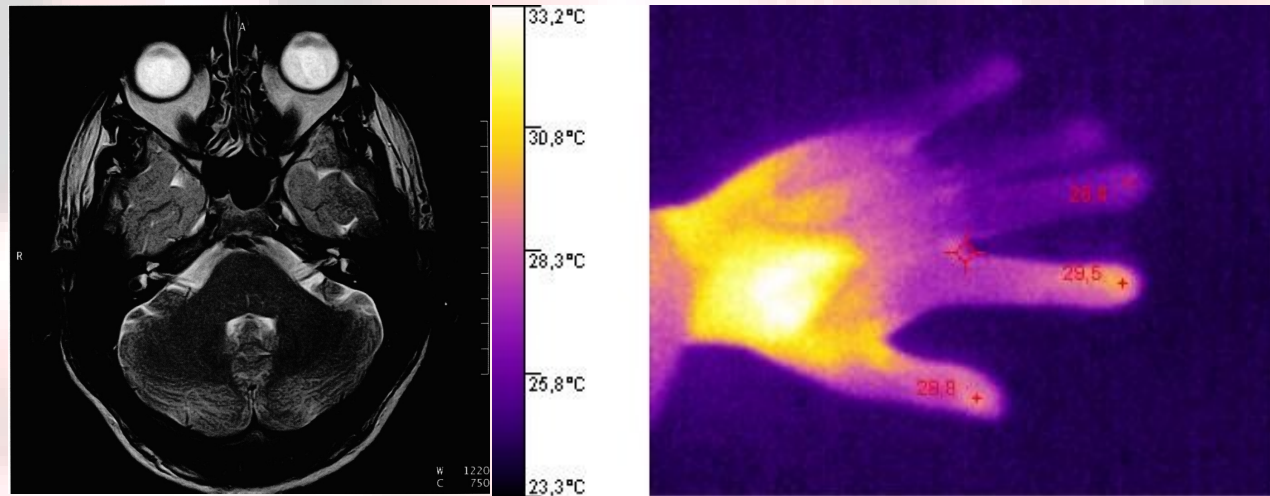

Magnetic resonance imaging (MRI)
Infrared imaging (thermography)

Magnetic resonance imaging

Infrared imaging

- The common feature of both imaging methods is the use of non-ionising radiation and the absence of genetic damage.
- Magnetic resonance imaging (MRI) is one of the most advanced imaging methods which gives both morphological and physiological (functional) information. The first MR image (cross-section of chest) was obtained by R. Damadian in 1977.
- Infrared imaging is a functional imaging method giving pictorial information on body surface temperature and thus level of metabolism. It is absolutely safe for the patient as the images are produced by IR radiation given out *by the patient himself*. First infrared cameras appeared in late 60' of 20th century.



MRI

Spin

- Spin is a specific property of sub-atomic particles (electrons, protons etc) like electric charge and mass
- Spin has some strange properties!
 - electrons, protons and neutrons all have the same spin i.e., $1/2$
 - pairs of particles of a single type (e.g., 2 electrons or 2 protons or 2 neutrons) can have a total spin of zero!
 - particles having non-zero total spin act like small magnets (we say they have a 'magnetic moment') and their energy is affected if placed in a magnetic field

Total Nuclear Spin (I)

- In MRI we are interested in the spin of NUCLEI
- In medicine, we use the magnetic properties of mainly light nuclides like **hydrogen** ^1H , phosphorus ^{31}P , carbon ^{13}C , fluorine ^{19}F or sodium ^{23}Na to get anatomical or physiological information.

Nuclide	Total Nuclear Spin I
H - 1	$\frac{1}{2}$
H - 2	0
C - 12	0
O - 16	0
N - 14	1
F - 19	$\frac{1}{2}$
P - 31	$\frac{1}{2}$
N - 15	$1\frac{1}{2}$

MRI Theory

- The magnetic moment μ of a nucleus is proportional to its angular momentum S ($\mu = \gamma \cdot S$, γ is **the gyromagnetic ratio**) which depends on I .
- In the absence of an external magnetic field, the magnetic moments of nuclei have all possible (random) directions with the result that:
 - The vector sum of the nuclear magnetic moments in a unit volume of a substance, i.e. the **magnetisation vector**, is equal to **zero**
 - The energy of all nuclei is the same


H Nuclei in a Uniform Magnetic Field B

- When *hydrogen* nuclei are placed in an homogeneous strong magnetic field with magnetic flux density B:
 - Their individual magnetic moments will precess with an axis parallel to the direction of B and orientate themselves either in the same direction or in the opposite direction to B
 - Therefore they have only two possible energies (a higher and a lower energy state).
 - The angular frequency of rotation of this precession (i.e., number of revolutions per second) - is called the **Larmor angular frequency** ω and is given by :


$$\omega = \gamma B$$

γ = gyromagnetic ratio


The H dipoles in the body precess at 42.6 MHz/T

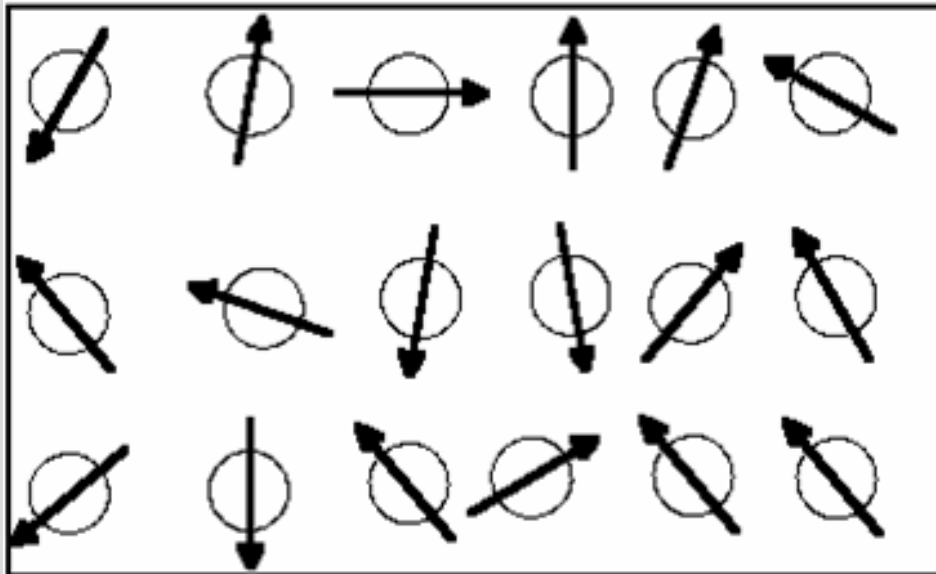

a) original state -
vectors of
magnetic moments
of nuclei are in
disorder, their
resultant equals
zero

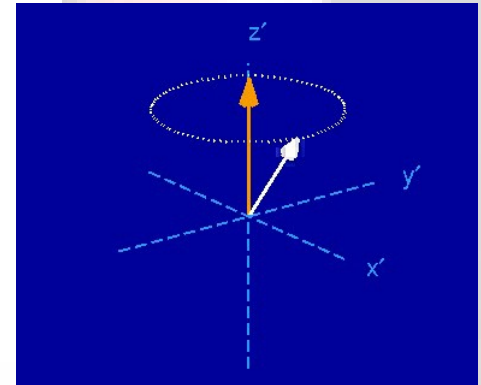


b) In a strong
magnetic field
with induction B
are magnetic
moments
oriented parallel
or antiparallel
with B

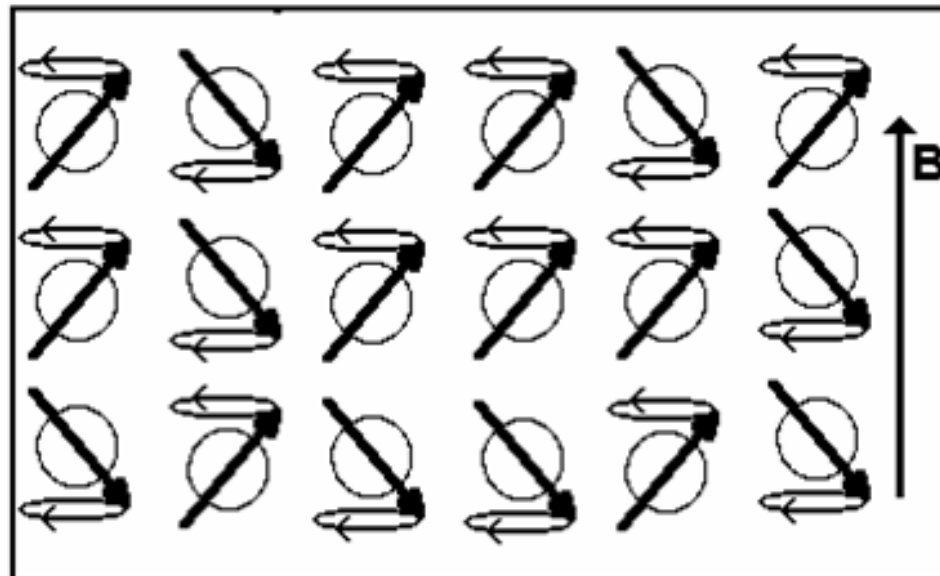

Video by Brian
Hargreaves,
Ph.D.

www-mrsrl.stanford.edu/~brian/mri-movies/

Magnetisation Vector

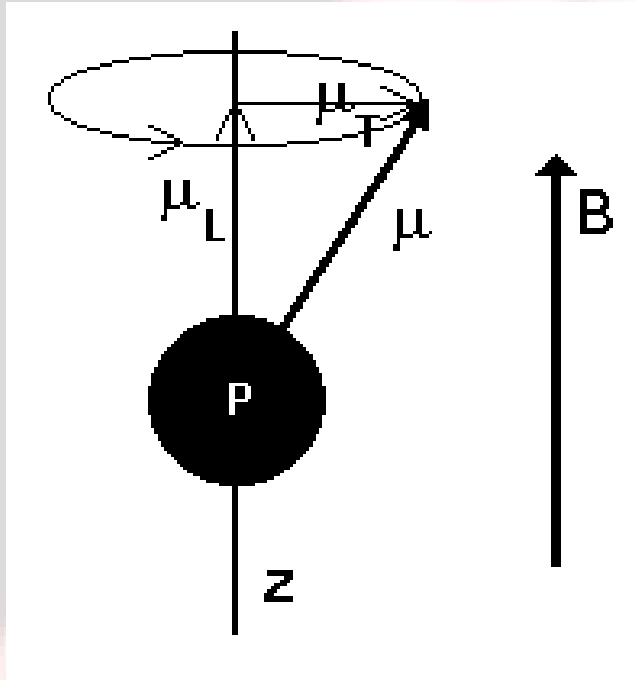

P - hydrogen nucleus (proton), B - magnetic flux density, z - axis identical with axis of precession (parallel with B), μ - magnetic moment of nucleus, μ_L - component of the magnetic moment of nucleus in z axis (vector sum of these projections in unit volume of a substance is the **longitudinal magnetisation vector**), μ_T - projection of μ in xy plane (vector sum of these projections in unit volume is the **transverse magnetisation vector**).

Measuring H Density in Tissues

For nuclei in the lower energy state to move to the higher energy state RF pulses of frequency equal to the Larmor frequency must be transmitted towards the patient using a transmitter coil (hence the 'resonance' in MRI). When this occurs the nuclei are also forced to precess in phase.

Longitudinal magnetisation vector becomes oriented in opposite direction

Transverse magnetisation vector appears and rotates in plane xy.

The return to the ground state (relaxation) is accompanied by the emission of a quantum of electromagnetic energy, which is when detected by an antenna (receiver coil) - the **nuclear magnetic resonance (NMR) signal**. The signal is relatively strong since the nuclei are precessing in phase. The amplitude of the pulse is proportional to the H density in the tissues (often known as 'spin density').

Relaxation times

- We have two **relaxation times**:
- **T_1 - longitudinal** - time necessary for return of the “population” of nuclei to the ground state. In biological media: 150 - 2000 ms.

Longitudinal magnetisation vector returns to original direction during this time.

T_2 - transversal - 2x - 10x shorter than T_1 . After this time interval the precession movement of individual nuclei is not in phase again.

Transverse magnetisation vector disappears after this time.

MRI - *Magnetic Resonance Imaging.*

- To recognize signals from the different parts of the patient magnetic field gradients („gradual change“) are used e.g., a gradient of B along the z-axis allows us to identify signals coming from different slices of patient perpendicular to the z-axis.
- The final image is produced using similar types of image generation processes as in CT.
- We can visualise differences in local hydrogen density or differences in relaxation times.

Technical aspects

- Up to values $B = 0.3 \text{ T}$ we can use giant permanent magnets (cheap but low contrast resolution).
- Electromagnets are stronger but need a lot of electric energy.
- Best contrast resolution but also the highest operational costs is obtained with **magnets having superconducting coil windings**, which can produce fields of up to $B = 10 \text{ T}$ today, but must be cooled by liquid helium. Typical values of B used in practice are $1 - 3 \text{ T}$.
- **Gradients** (about several $\text{mT}\cdot\text{m}^{-1}$) of magnetic field are formed by additional coils.

MR Contrast and MR Spectroscopy

- Some paramagnetic atoms can amplify the signal. That is why e.g., **gadolinium** is used as a contrast agent for MRI. Gadolinium is chemically bound to certain pharmaceuticals e.g., DTPA - diethylen-triamin-penta-acetic acid.
- The exact value of the Larmor frequency changes slightly (shifts) according to the position of the hydrogen in the molecules. For example, different shifts of H in groups =CH- or -CH₂- are well measurable. This allows us to identify such groups using **in-vivo MR - spectroscopy** is a powerful tool with application in functional MRI (analysis of ATP content etc.)

Safety aspects

- The magnet can impair function of other medical devices. Hence MRI is strongly contraindicated in patients with some electronic devices inside their bodies (pacemakers, cochlear implants etc.)
- Iron objects are strongly attracted to the “*gantry*” – they can damage the device and cause injuries. MRI is strongly contraindicated in patients with any iron bodies inside (implants, bullets, splinters of grenades etc.)
- MRI is not recommended in the first trimester of pregnancy.
- Some minor problems can be caused by any metals inside the body or on the body surface (heating, prickling sensations). For example: jewellery, some mascaras, old tattoos, tooth fillings, dental crowns and frameworks, implants etc.)
- Some patients are anxious or unquiet inside the device gantry, because of strong noise during the examination. Claustrophobia is also common.

Important Advice

magnetic memories (e.g., credit cards) can be destroyed if taken into an MRI room

MRI Devices



„T2 weighted“ image of transversal section of head in the level of cochlea.

(Siemens).



MR - Angiogram



BMRI @ J.Hornak

Sagittal section of cervical spine





Sagittal section of knee



3D model of curvature of left *A. cerebri media* (arrow) and M1 segment of the same artery (wedge)

B) other view on this model shows also curvature of *A. cerebri media* (arrow shows a well visible aneurysm)

These are not plastic models but the result of real MRI image processing!

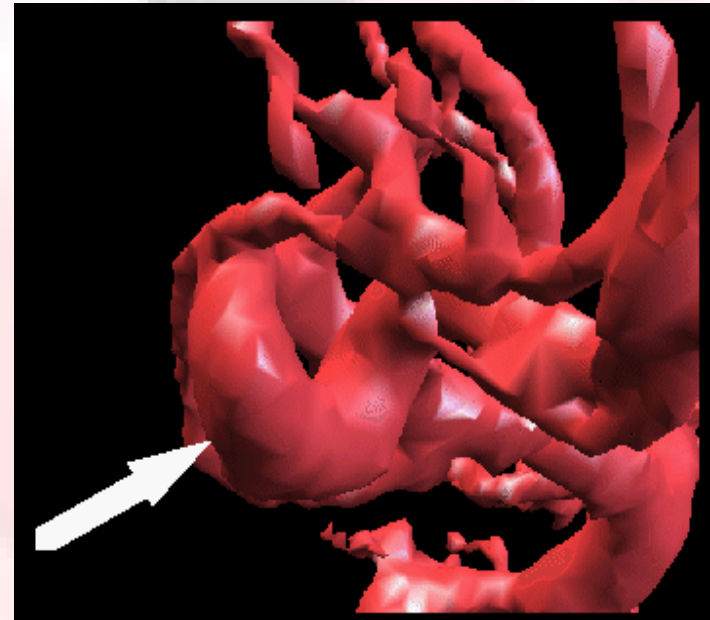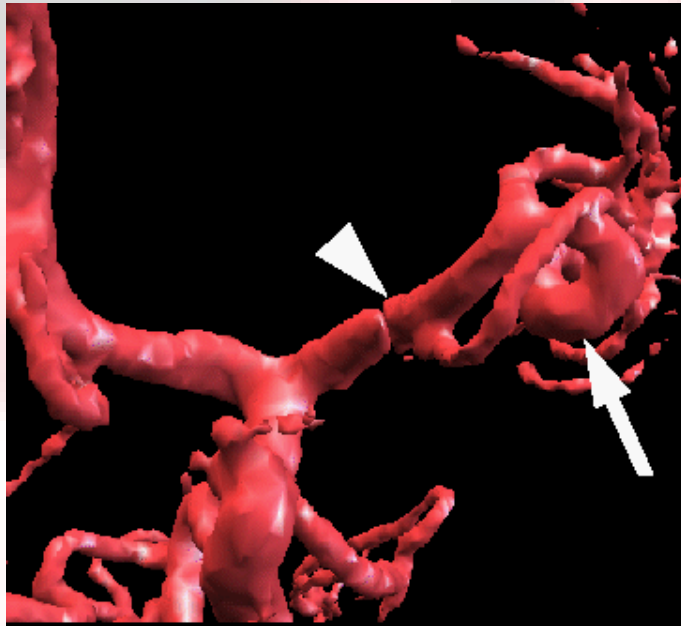

The background of the slide is a blurred image showing several hands holding a device, possibly a smartphone or tablet, in a way that suggests a collaborative or shared activity. The image is out of focus, with the hands and the device appearing as soft, light-colored shapes against a darker, muted background.

Thermography

What is infrared imaging and infrared radiation?

- The contact-less thermographic method is based on the measurement of infrared radiation (IR) emitted by the surface of the body.
- Digital sensor technology is used for image recording.
- Wavelength 780 nm - 1 mm
- IR visualised first by Holst in 1934
- Discovered by astronomer Herschel in 1800
- The wavelength used in thermography 0.7 - 14 μm

Principle of image recording

A digital camera with an IR-sensitive pixel sensor array (microbolometer).

Microbolometer is a grid of vanadium oxide or amorphous silicon heat sensors atop a corresponding grid of silicon. IR radiation from a specific range of wavelengths strikes the vanadium oxide and changes its electrical resistance. This resistance change is a measure of the temperature. Temperatures can be represented graphically. The microbolometer grid is commonly found in many sizes e.g., 244 x 193 (Meditherm), 160×120 array (Fluke).



Meditherm Med2000®

Maximizing the potential of thermography

Meditherm Med2000 Specifications For Standard Clinical Applications

Camera

- Coolant: Thermoelectrically cooled
- Weight: 2 kg
- Size: 14cm W x 43cm H x 11cm D
- Operating Temperatures: 10°C to 37°C

Image display


- 10 x True colour palettes
- 1 x 16-step grayscale.
- 3 x 16-step Isotherm.
- Dynamic range: 24 bits
- Image stored in TIF format
- Image size 95kb
- Temperature step sizes: 0.1 - 2°C

Image Acquisition

- Temperature ranges:
10°C to 40°C (Standard Calibration)
- Thermal sensitivity: < 0.01°C
- Field of view: 30.5° x 22.5°
- Spatial resolution:
0.4 mm (camera at 15 cm)
1mm (camera at 40 cm)
- Resolvable elements: 244 x 193 pixels
- Image scan rate: 8 seconds (47K pixels)
5 seconds (23.5K pixels)
- Emissivity correction: User variable
0-100% default setting 100%

IR camera of Dept. Of Biophysics, Faculty of Medicine, MU, Brno

Fluke Ti30

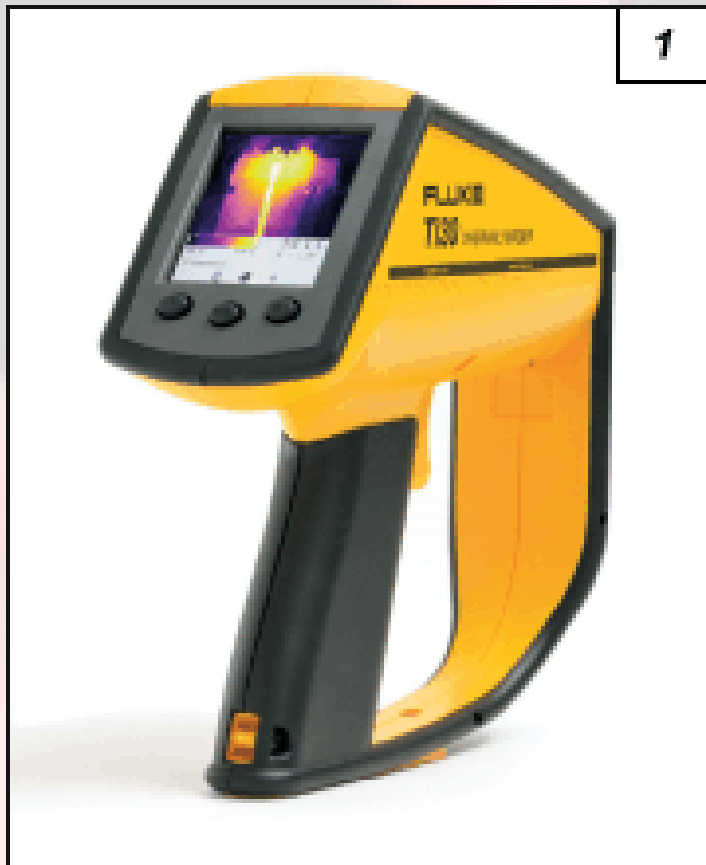

Accessories



IR imaging in medicine – advantages and disadvantages

- High temperature and spatial resolution
- Temperature distribution is displayed in the form of isothermal lines - isotherms
- Possibility to display temperature profiles
- Fast measurement

- **Surface temperature distribution differs even in healthy people**
- **We have always to compare temperature of symmetrical body parts**
- **In contrast to original expectation, it is not possible to use IR imaging as a screening method for malignancies, e.g. breast tumours, because of its low specificity.**

Clinical Importance of Thermography

The method informs us about the extent and dynamics of any pathological process which is accompanied by increased temperature.

Indications

- Diseases of peripheral blood vessels
- Diseases of thyroid
- Diseases of lymphatic system
- Joint inflammations
- Demarcation of burns and frostbites
- Assessment of blood supply after reconstruction surgery...

Imaging conditions:

Temperature of darkened room 20 °C

Acclimatisation time about 20 min.




Examined body area must be uncovered during acclimatisation

It is not allowed to smoke, drink alcoholic beverages, exercise or take drugs causing vasodilatation or vasoconstriction before examination


A blurred background image showing a group of people holding hands in a circle, symbolizing unity and support. The image is out of focus, with the hands and arms appearing as soft, light-colored shapes against a darker background.

Clinical Thermograms



Different palettes of colours (Fluke)

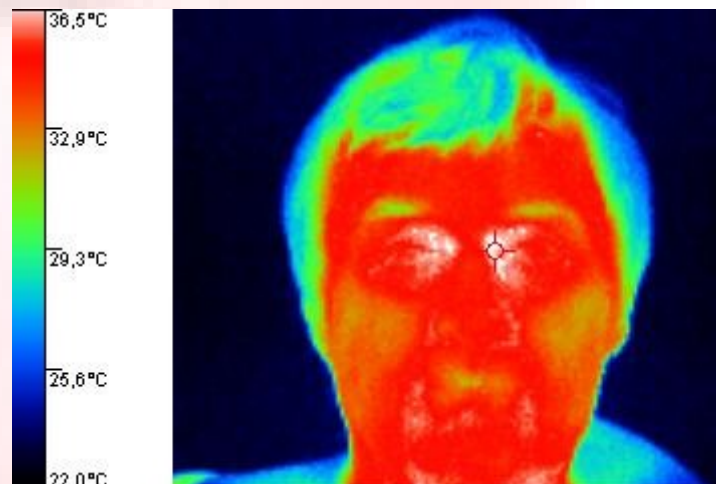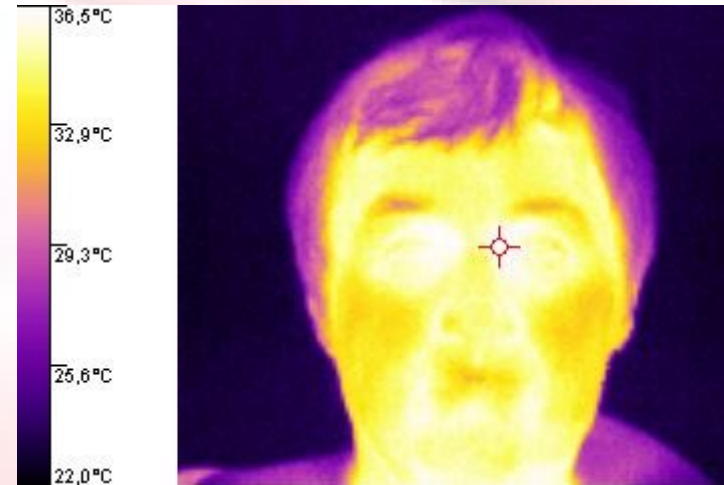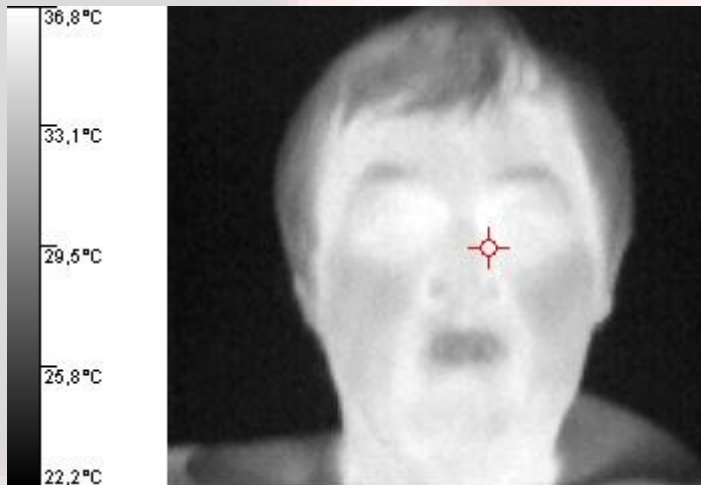


Human face (Fluke)

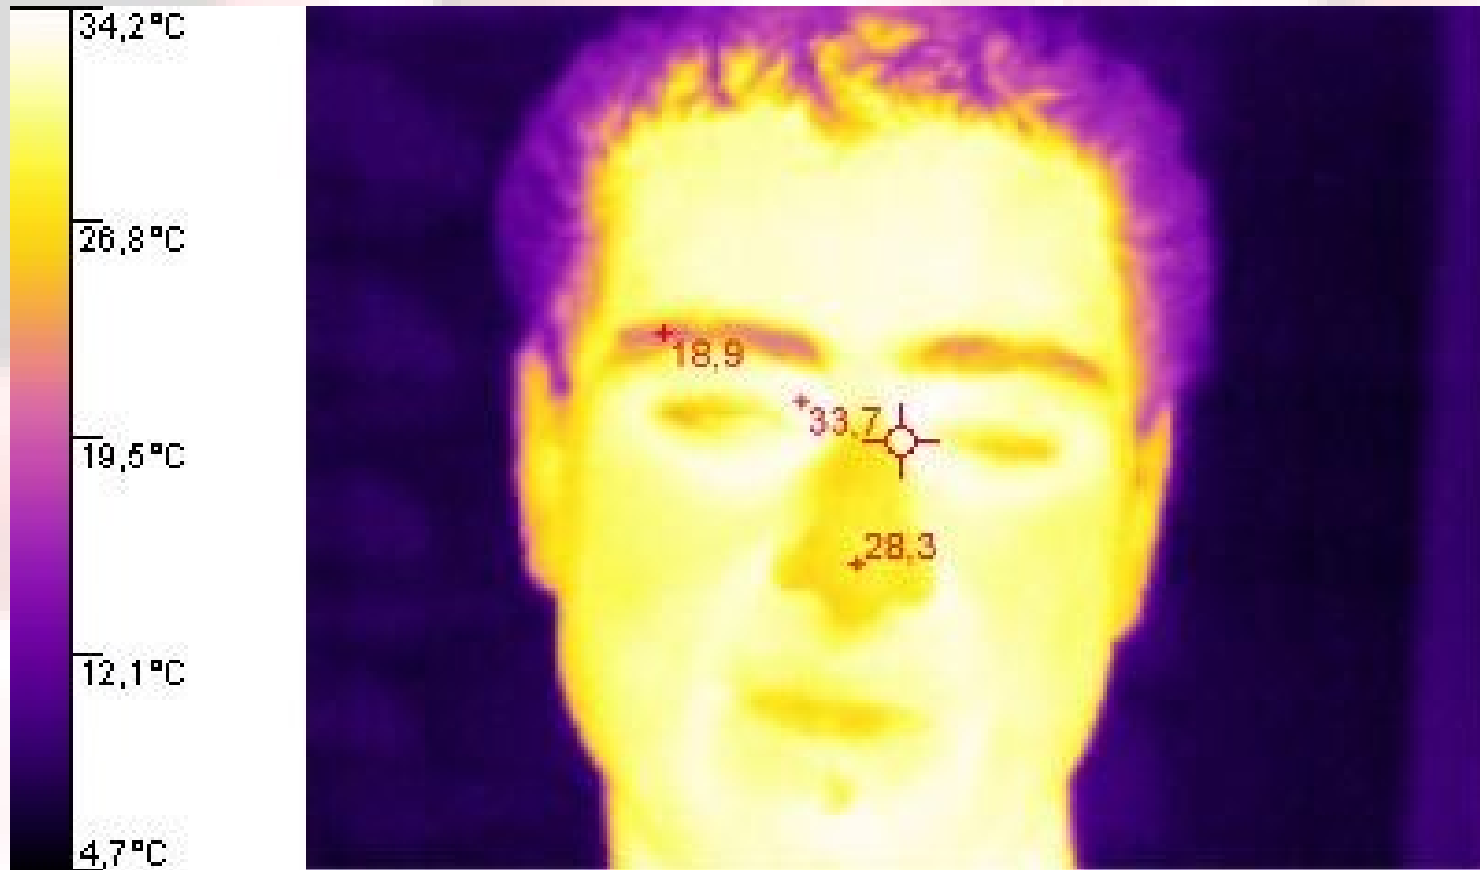

Thermogram of fingers before and after cold test (Fluke)

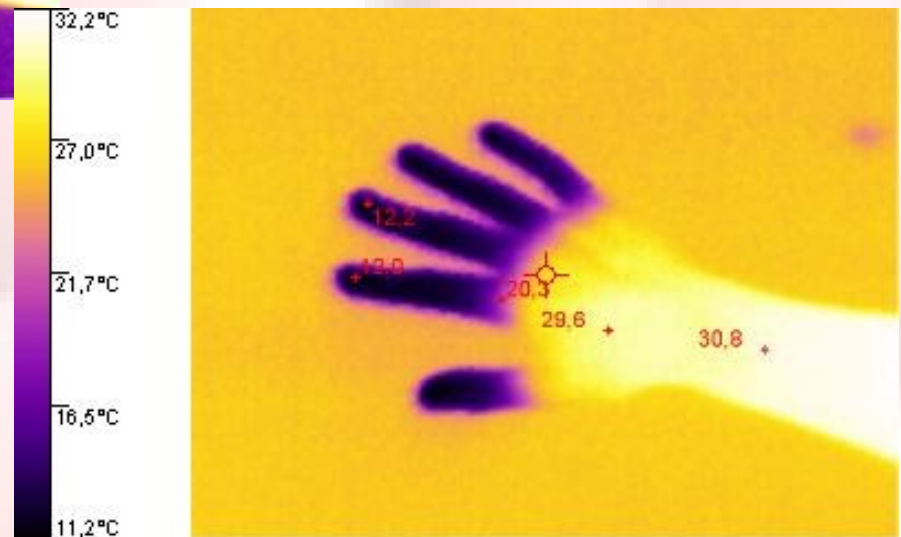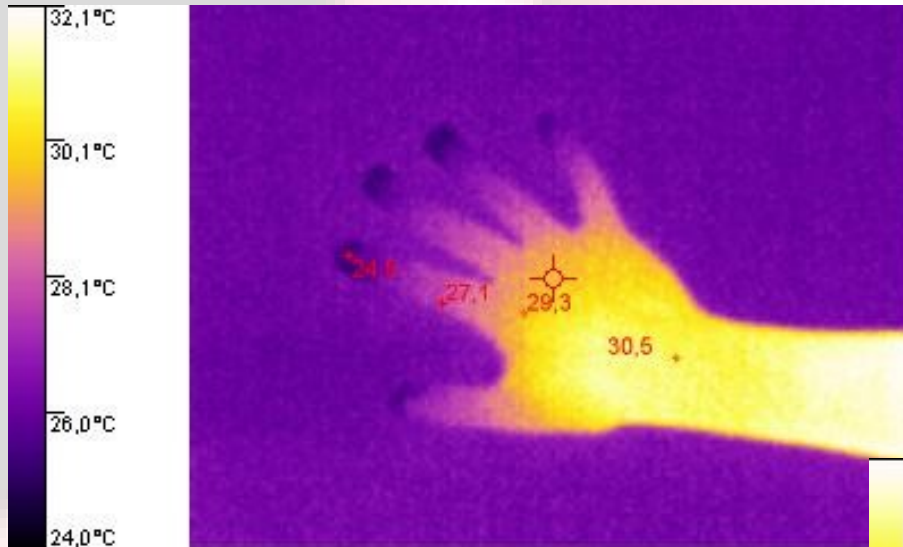

Finger inflammation after a small injury (FLUKE Ti30)

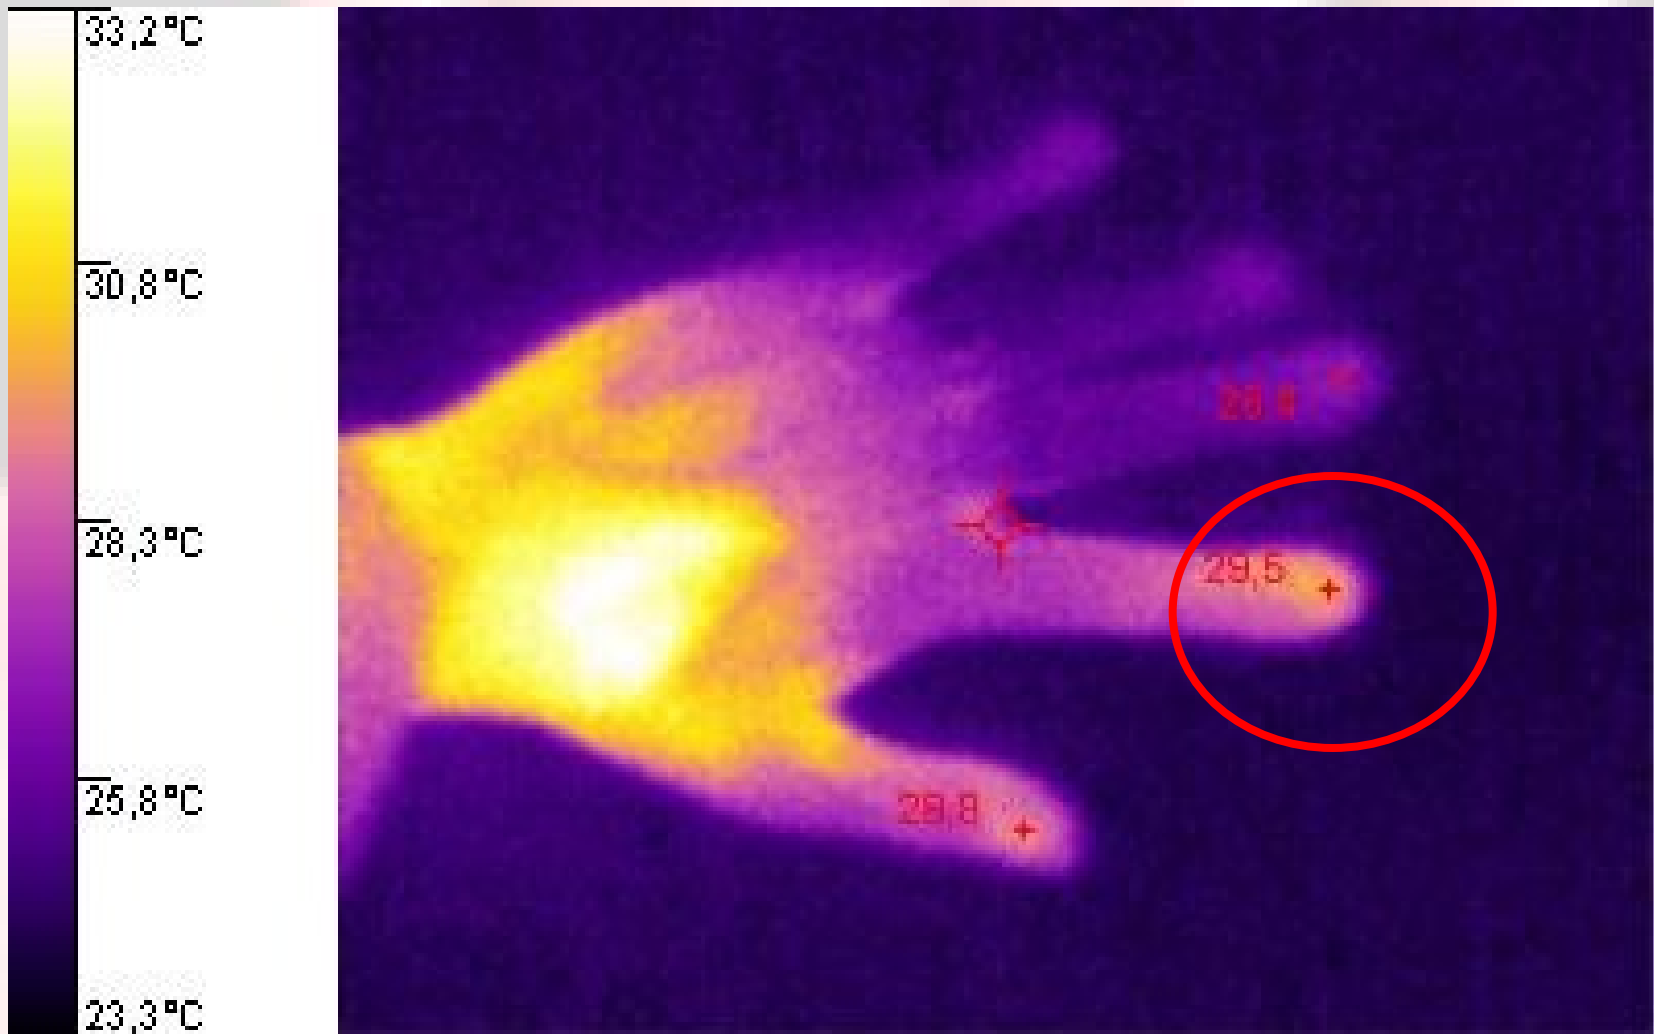

Varicosity of lower limbs (Fluke)



Knee inflammation




Myofascial Trigger Point Upper Right Levator Scapula

Diffuse Patterns Of Hyperthermia Over Central Spine


Cervical Inflammation




Isotherm Palette

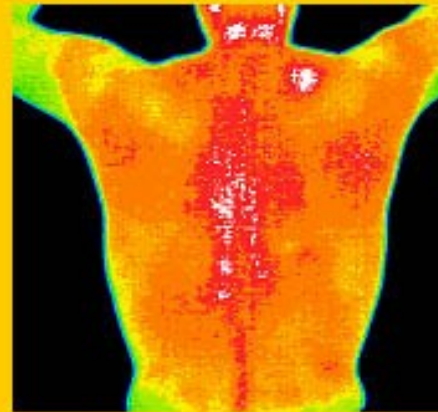


Standard Color Palette

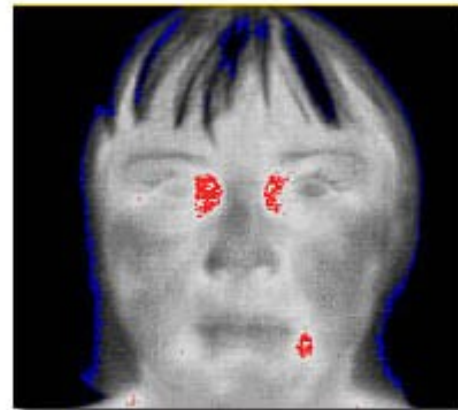

www.mhs5000.com/software.htm

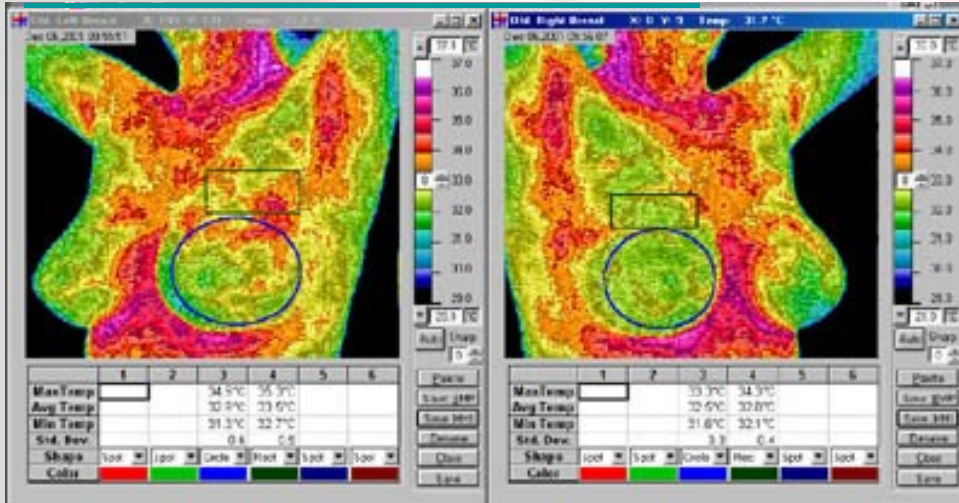

**Stress fracture on football player
X-ray showed no abnormality, thermography correlated well with the patients report of pain and provided justification for the more invasive test of scintigraphy which clearly showed a stress fracture in the exact location indicated by the thermogram.**

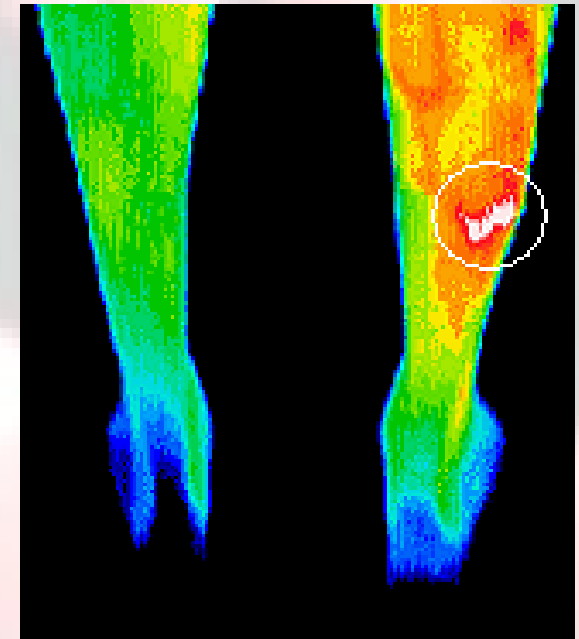


www.dititexas.com/page6.html



Use of the IR Camera for Safety Studies


Oven leaking heat – checking heat devices

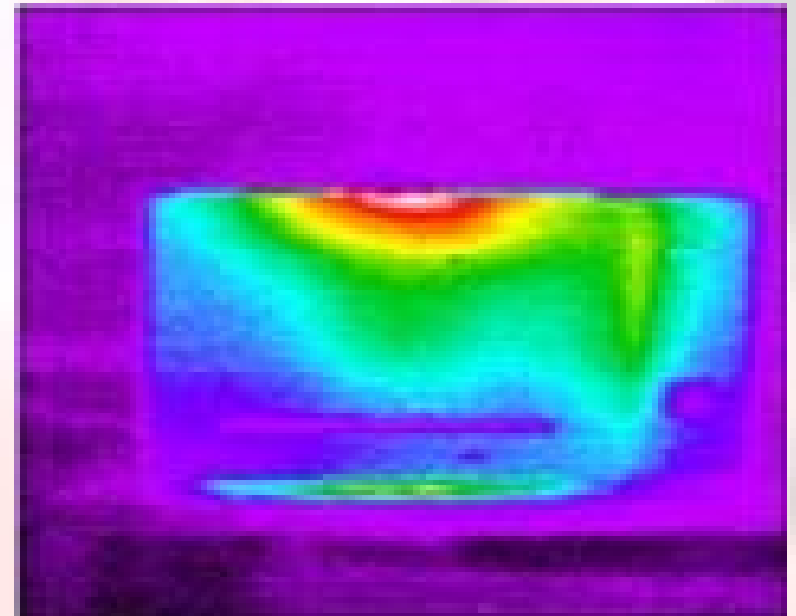


Overheated cable



Low quality insulation of a warm water piping in area of joints (Fluke)

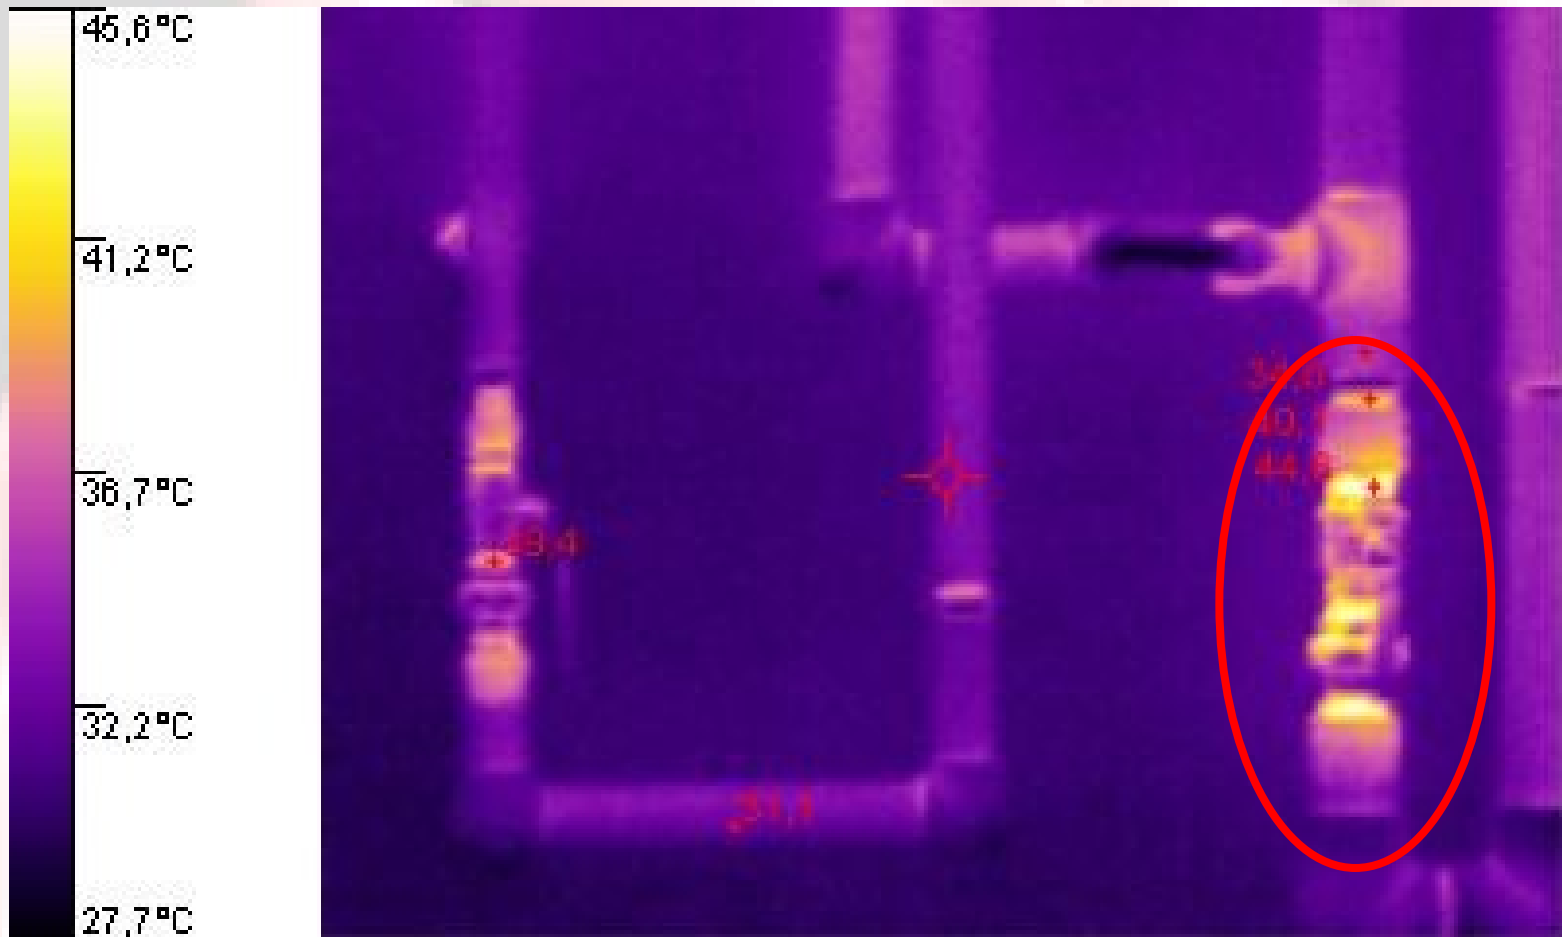


Ultrasonographic probe (Fluke)

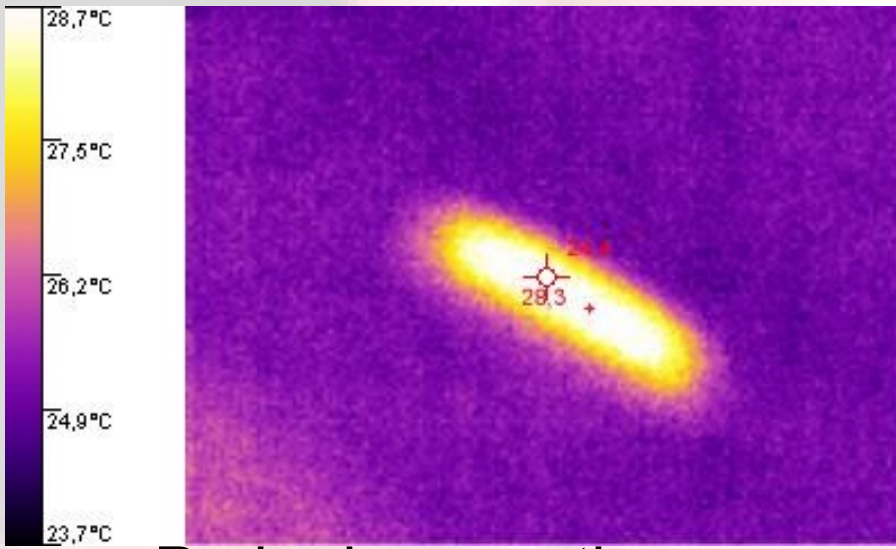


Probe in operation
28,3 C


Probe „frozen“
26,5 C

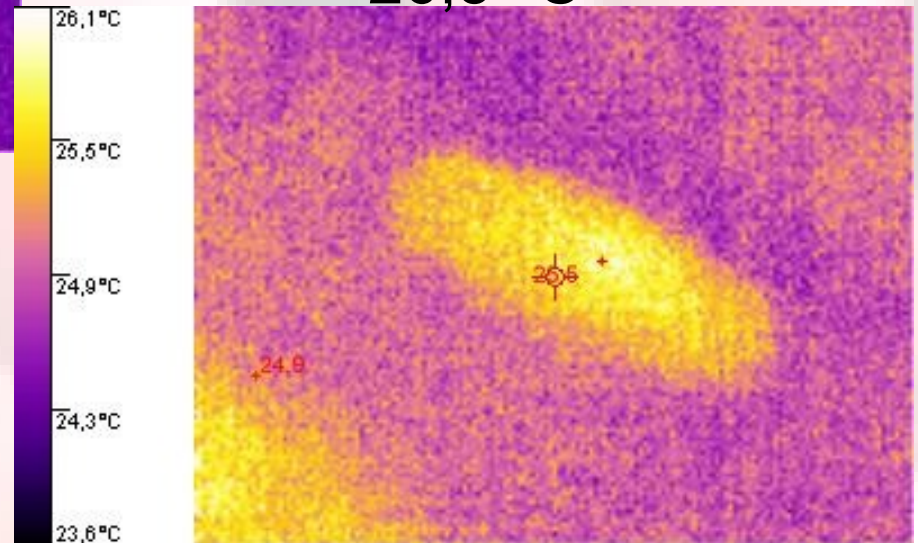

Thermal spot left by ultrasonographic probe on the forearm + cooling effect of the coupling gel (Fluke)

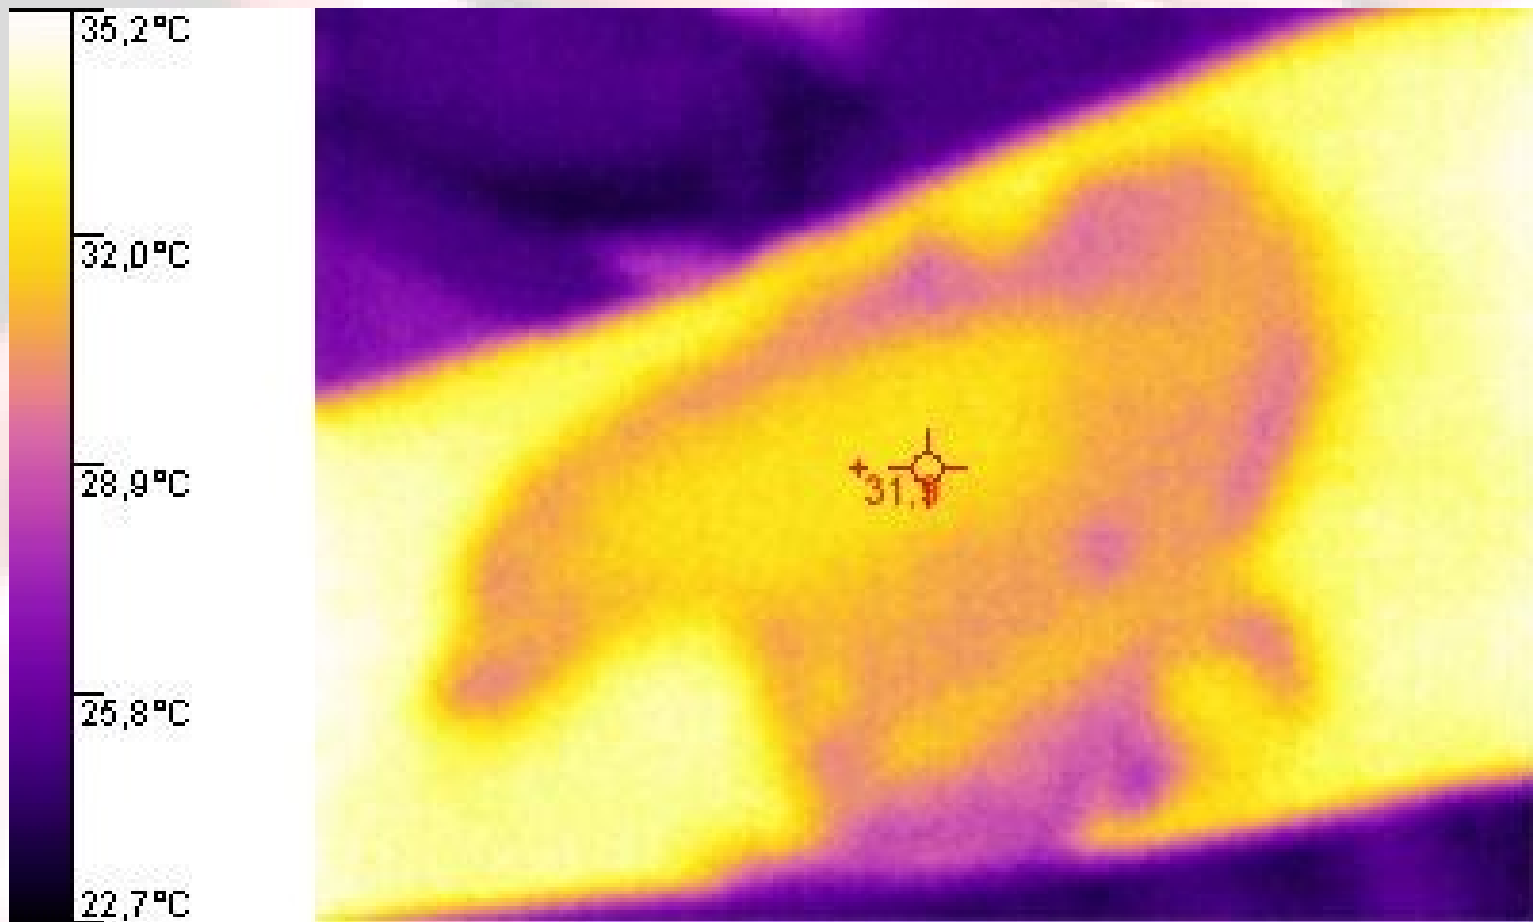

Ultrasound therapy application head (Fluke)

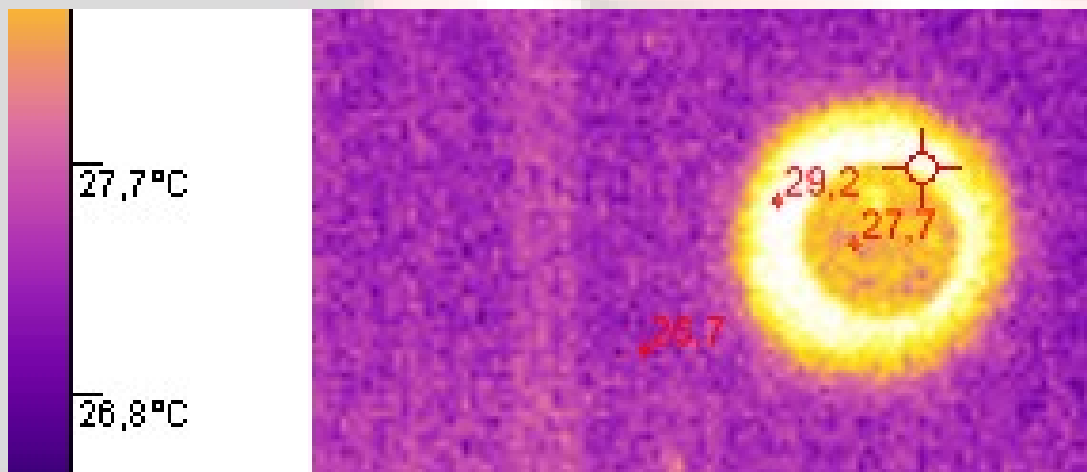


Intensity $0,5 \text{ W/cm}^2$

Head temperature 27,7 °C.

Head rim temperature 29,2 °C

Surrounding area 26,7 °C

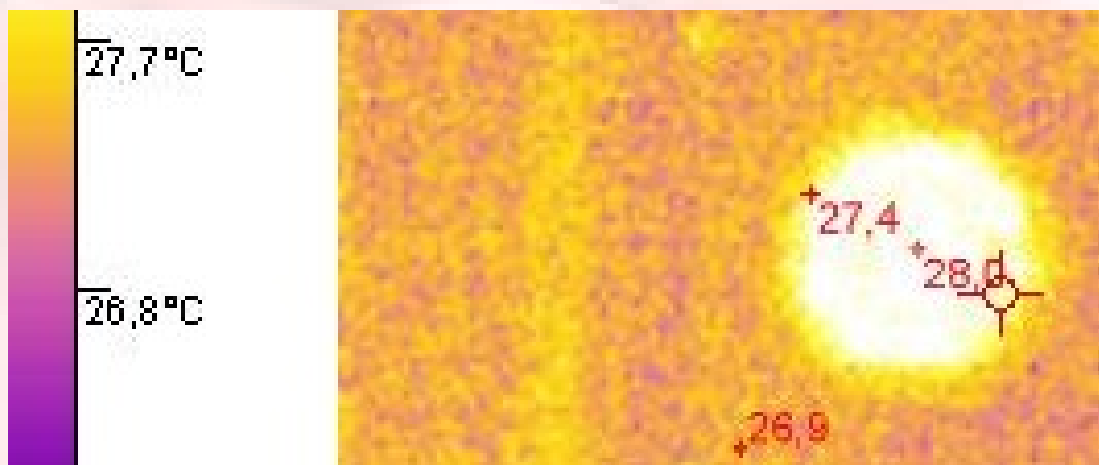

Intensity 2 W/cm^2

Head temperature 28 °C

Head rim temperature 27,4 °C

Surrounding area 26,7 °C

Authors:

**Vojtěch Mornstein Carmel J. Caruana,
Ivo Hrazdira**

Last revision: May 2009

Last revision: May 2009

Carmel J. Caruana

Language revision:

Lucie Mornsteinová

Presentation design: