

How to divide respirators?



Classification of respirators in the EU

-evel			
FFP1	Dust protection		
FFP2	Protects against solid and liquid dusts, aerosols and fumes harmful to health. Filters at least 94% of aerosols down to 0.6 μ m.	FFP2	
FFP3	Protects against solid and liquid dusts, aerosols and fumes harmful to health. Filters at least 99% of aerosols (airborne particles) down to 0.6 μ m.	FFP1 94%<	

Classification from CDC webside (for USA):

https://www.cdc.gov/niosh/np ptl/topics/respirators/disp_par t/default.html

N95 – Filters at least 95% of airborne particles. Not resistant to oil.

(N95 Manufacturers Index: <u>3M A B C D E F G H I J K L M N O P Q R S T U V W X Y Z</u>)

<u>Surgical N95</u> – A NIOSH-approved N95 respirator that has also been cleared by the Food and Drug Administration (FDA) as a surgical mask.

N99 – Filters at least 99% of airborne particles. Not resistant to oil.

N100 - Filters at least 99.97% of airborne particles. Not resistant to oil.

R95 - Filters at least 95% of airborne particles. Somewhat resistant to oil.

P95 - Filters at least 95% of airborne particles. Strongly resistant to oil.

P99 – Filters at least 99% of airborne particles. Strongly resistant to oil.

P100 – Filters at least 99.97% of airborne particles. Strongly resistant to oil.

Certification Name	N95	FFP2	KN95	P2	KF94 (Korea 1st Class)	DS2	PFF2
Standard	NIOSH-42 CRF 84	EN 149-2001	GB2626-2006 (updated to GB2626-2019)	AS/NZ 1716:2012	KMOEL-2017-64	JMHLW Notification 214, 2018	ABNT/NBR 13.698.2011
Locality	United States	European Union	China	Australia & New Zealand	South Korea	Japan	Brazil
Filtration Performance	≥ 95%	≥ 94%	≥ 95%	≥ 94%	≥ 94%	≥ 95%	≥ 94%
Flow Rate	85 L/min	95 L/min	85 L/min	95 L/min	95 L/min	85 L/min	95 L/min
Total Inward Leakage (tested on human subjects)	N/A	≤ 8% leakage	≤ 8% leakage	≤ 8% leakage	≤ 8% leakage	Inward Leakage included in individual device's instructions	N/A
Inhalation Resistance	≤ 343 Pa (at 85L/min)	≤ 70 Pa (at 30 L/min) ≤ 240 Pa (at 95 L/min) ≤ 500 Pa(clogging)	≤ 350 Pa (at 85 L/min)	≤ 70 Pa (at 30 L/min) ≤ 240 Pa (at 95 L/min)	≤ 70 Pa (at 30 L/min) ≤ 240 Pa (at 95 L/min)	≤ 70 Pa (w/valve at 40 L/min) ≤ 50 Pa (novalve at 40 L/min)	≤ 70 Pa (at 30 L/min) ≤ 240 Pa (at 95 L/min)
Exhalation Resistance Pressure Drop	≤ 245 Pa (at 85L/min)	≤ 300 Pa (at 160 L/min)	≤ 250 Pa (at 85 L/min)	≤ 120 Pa (at 85 L/min)	≤ 300 Pa (at 160 L/min)	≤ 70 Pa (w/valve at 40 L/min) ≤ 50 Pa (no valve at 40 L/min)	≤ 300 Pa (at 160 L/min)

• https://breathesafeair.com/mask-ratings/

Procedure Masks

Disposable **procedure** masks are widely available. They are sometimes referred to as surgical masks or medical procedure masks.


Wear procedure masks with

- · A proper fit over your nose, mouth, and chin to prevent leaks
- Multiple layers of non-woven material
- A nose wire



Do NOT wear procedure masks with

- Gaps around the sides of the face or nose (see example)
- · Wet or dirty material

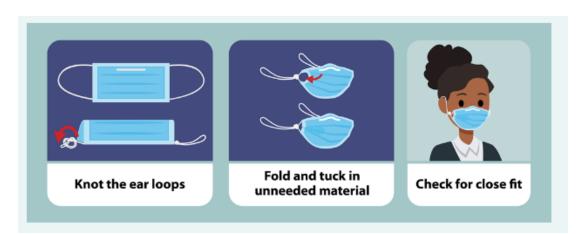



Zdroj: https://www.cdc.gov/coronavirus/2019-ncov/prevent-getting-sick/types-of-masks.html

Respirators


What to know about international respirators:

- They are designed to standards that do not often have a quality requirement.
- They filter varying levels of particles in the air depending on the standard they are designed to meet.
- They seal tightly to your face when fitted properly.
- It is important to pick a respirator that fits your face and seals well since not all fit the same.

Do NOT wear international respirators:

- If they have exhalation valves, vents, or other openings
- If it is hard to breathe while wearing them
- If they are wet or dirty
- With other masks or respirators
- As a replacement for NIOSH-approved <u>respiratory protection when required by your job</u>

https://www.cdc.gov/coronavirus/2019-ncov/prevent-getting-sick/types-of-masks.html

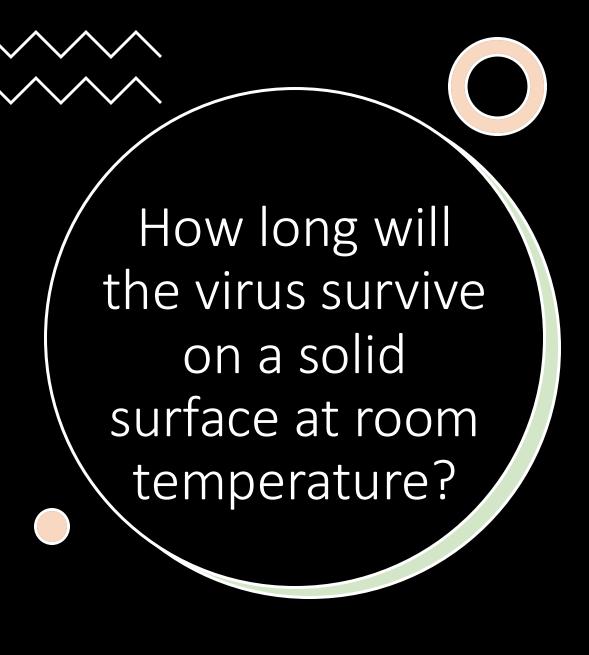



 After the transition to practice - where will you look for information on changes or innovations to the hygiene regime in dental office?

• CDC

- WHO
- Professional dental and dental hygiene societies