Roentgen tube – x- ray tube:

Cathode – Anode – Tension



Catode (heated) - Electrons – go against Anode – brake - x ray originates

 Imaging method completing clinical examination of patients

Principle:


X- rays going through various materials (tissues) are absorbed – image on the film (a special suspension AgBr – silver bromide)

Roentgen tube X ray tube

Cathode
wolfram
(tungsten) filament inside
(heated – brought to white heat)

Focus – made of wolfram

Anode -

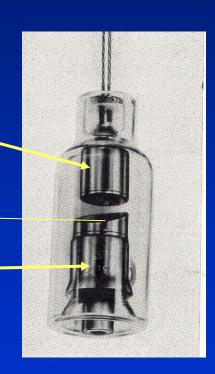

Extraoral and intraoral radiography

Extraoral:

The film is placed outside of oral cavity


- OPG (orthopantomography)
- Teleradiography
- Special projections of a skull (posteriorly anteriorly)
- Half axial
- Side projection (TMJ, mandible)
- CT

Extraoral and intraoral radiography


Intraoral – the film is placed into the oral Cavity – a special x-ray apparatus.

- Teeth
- Alveolar bone
- Periodontal space
- Fillings
- Caries
- Level of endodontic treatment



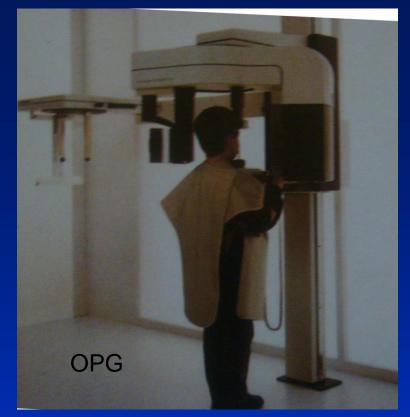













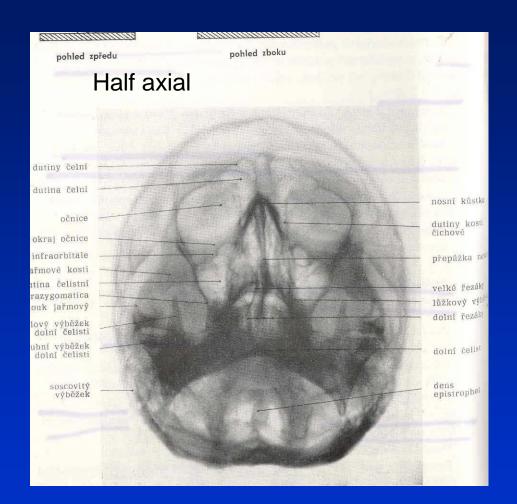

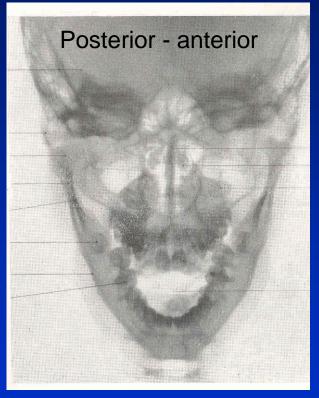

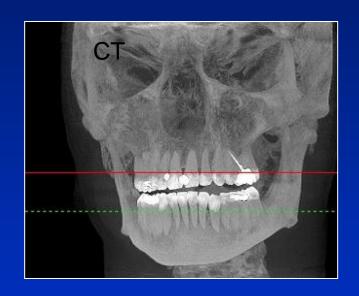

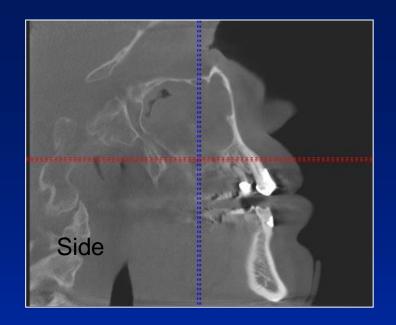



Intraoral radiography

Film or sensor placed in oral cavity Special apparatus


- Teeth
- Alveolar bone
- Periodontal space
- Fillings
- Caries
- Impacted teeth
- Level of endodontic treatment





Parallel technique Film or sensor in a special holder Parallel to long axis of teeth




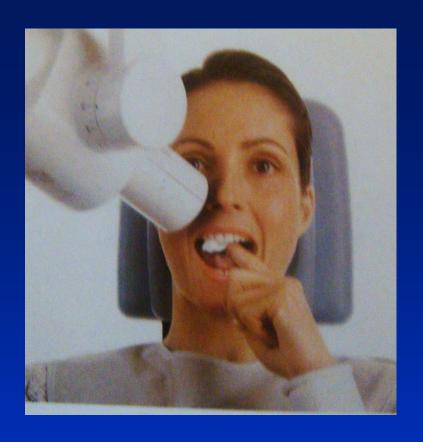

Techique of isometric and orthoradial radiogram




Technique of halving angle – isometric radiogram

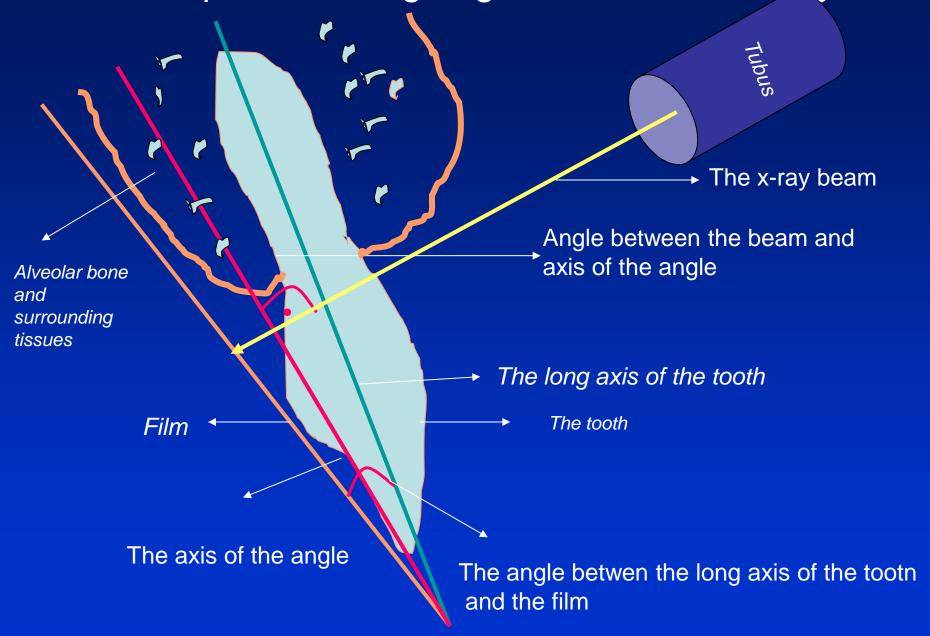

Hypometric and hypermetric picture

Hypometric – the picture is smaller


Central beam goes perpendiculary on the tooth





Hypermetric picture – the picture is bigger

- central beam goes perpendiculary to the film paprsek jde kolmo na film.





The tubus can have vairous position

Apical projection: the central beam goes through the apex area

 Periodontal projection: the central beam goes through the uper third of the root


 Coronal projection: the central beam goes through the crown.

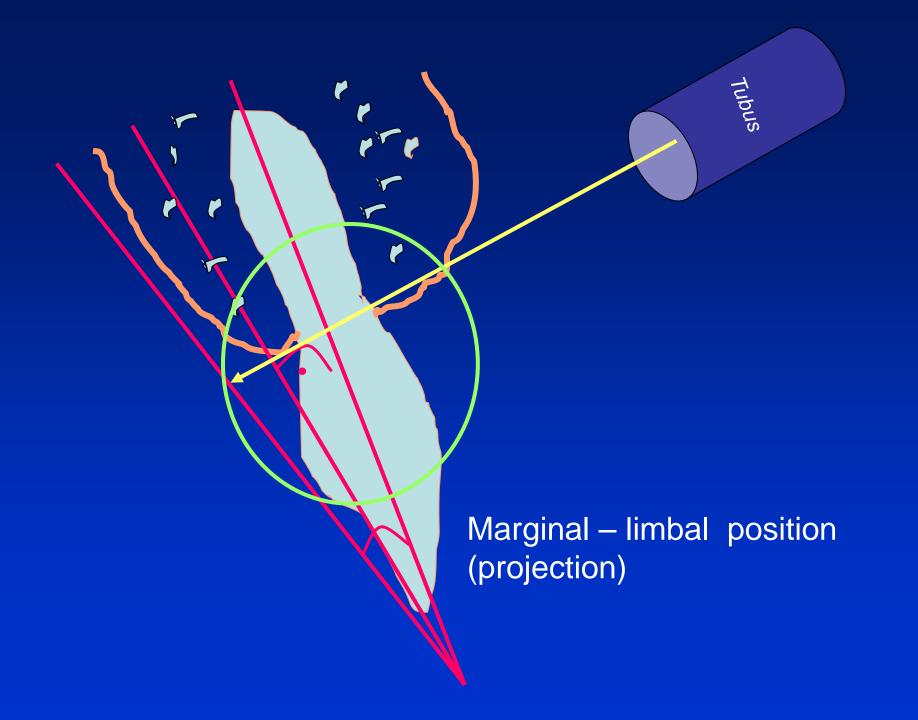


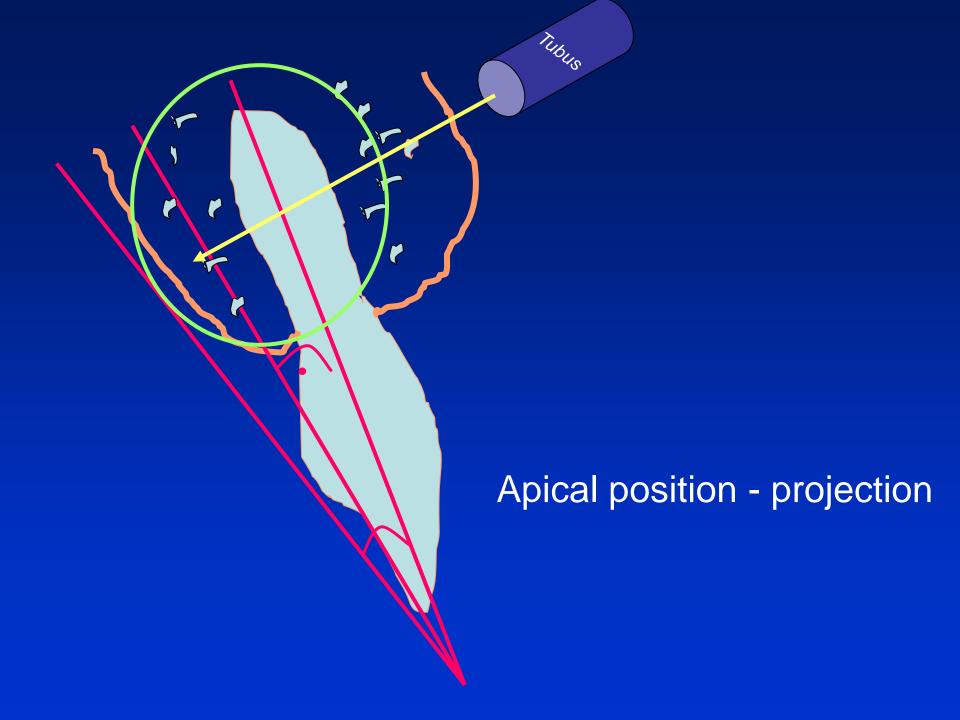

Orthoradial and excentric projektion

- Orthoradial the central beam goes parallel to interdental septa
- Excentric
 — the central beam goes from distal or mesial side.

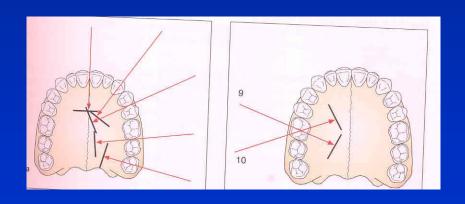



Bitewing





Fiml or sensor is in a special holder, patien bites into
Tje central beam goes parallel to interdental septa
Crowns of teeth are well seen – good for early diagnosis of dental caries







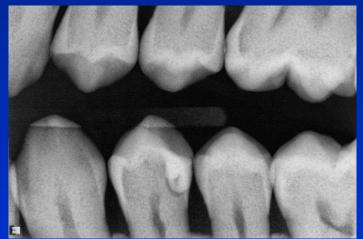

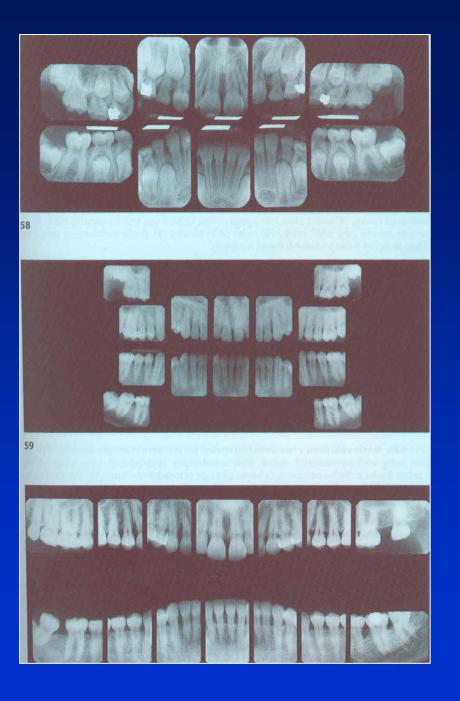


Rtg status



OPG



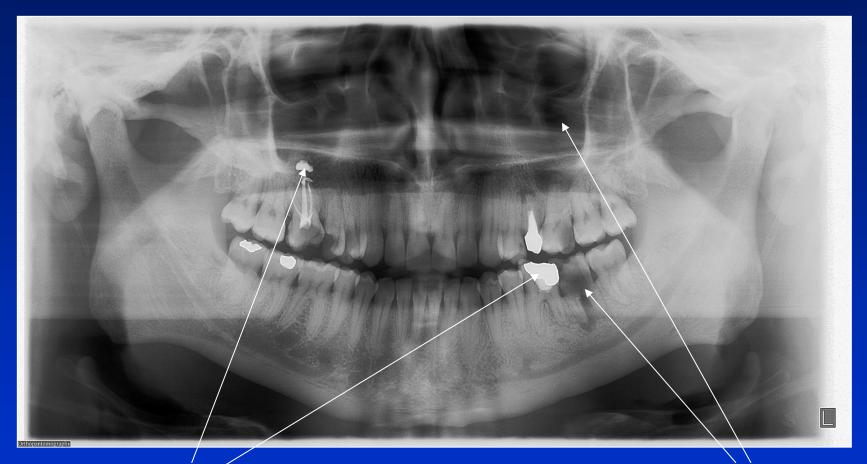


radioopacity

radiolucency





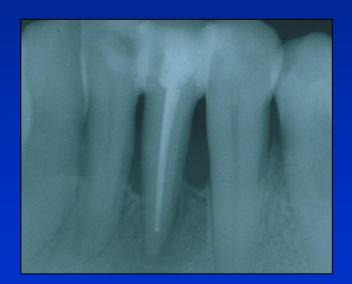



i.o.

