

Ultrasound in endodontics

Endodontics

- Location of the root canals
- Root canal shaping
- Activation of irrigation
- Removal of broken root canal instruments
- Apical surgery












Endodontics


Activation

Movement of liquid

Cavitation

Sonolysis

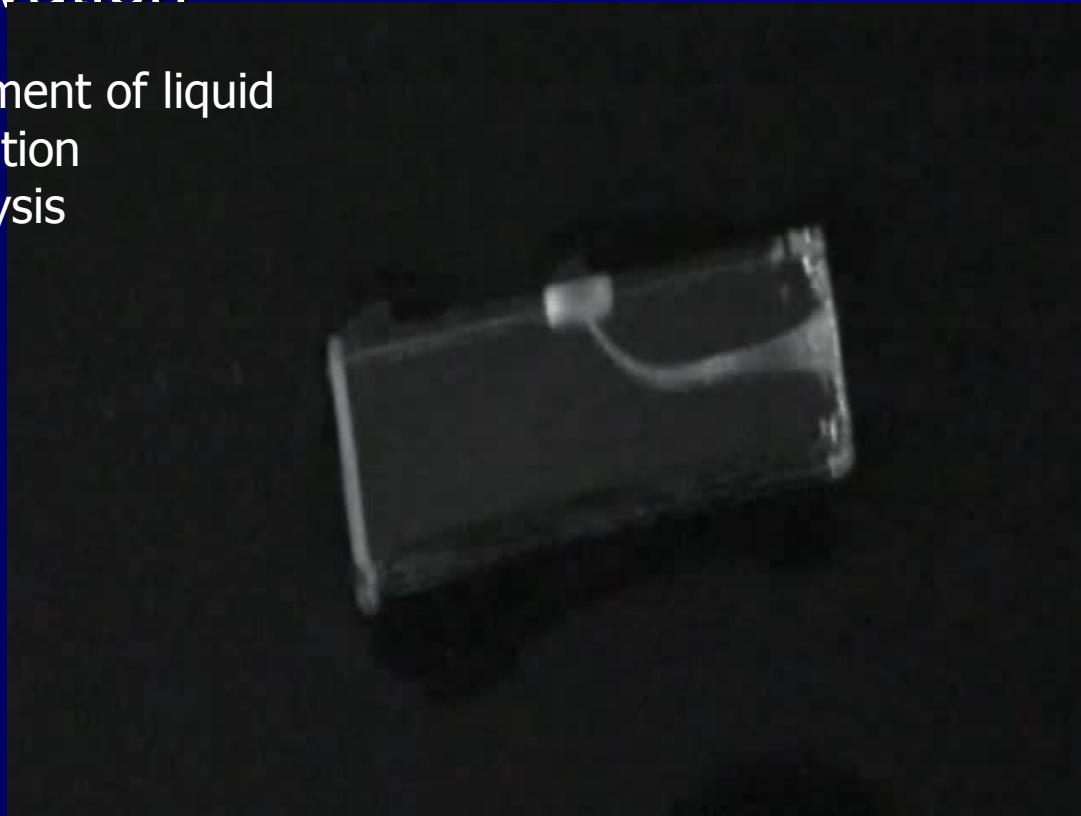

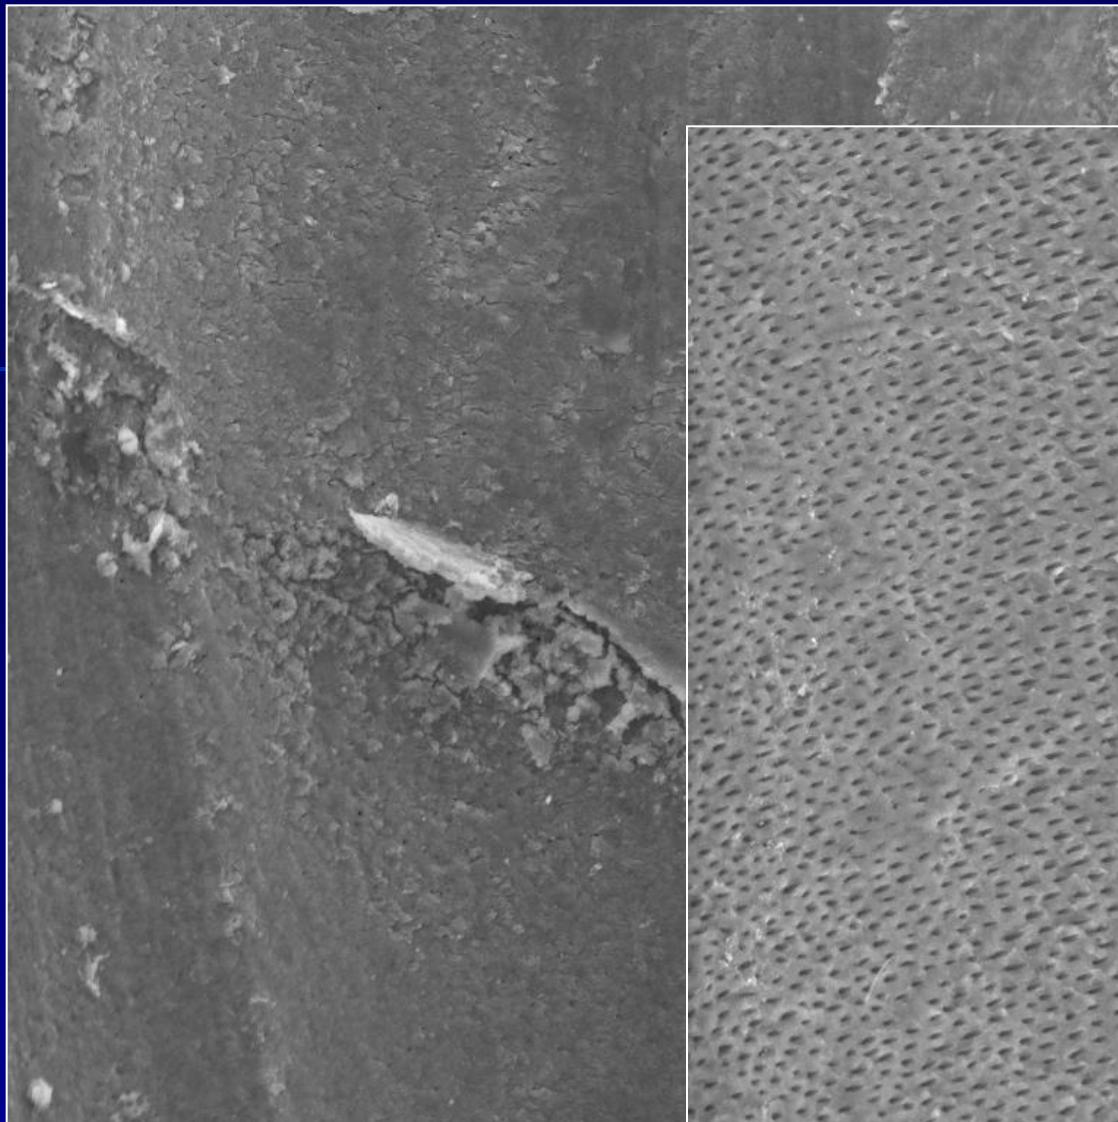

SEM MAG: 535 x DET: Ionizační
HV: 25.0 kV PC: 13
VAC: LowVac, 514 Pa Scan speed: 6

200 um
Digital

SEM MAG: 581 x DET: Ionizační
HV: 25.0 kV PC: 13
VAC: LowVac, 519 Pa Scan speed: 6

100 um


Vega ©Tescan

Digital Microscopy Imaging AQUASEM-VEGA





Removal of broken instruments

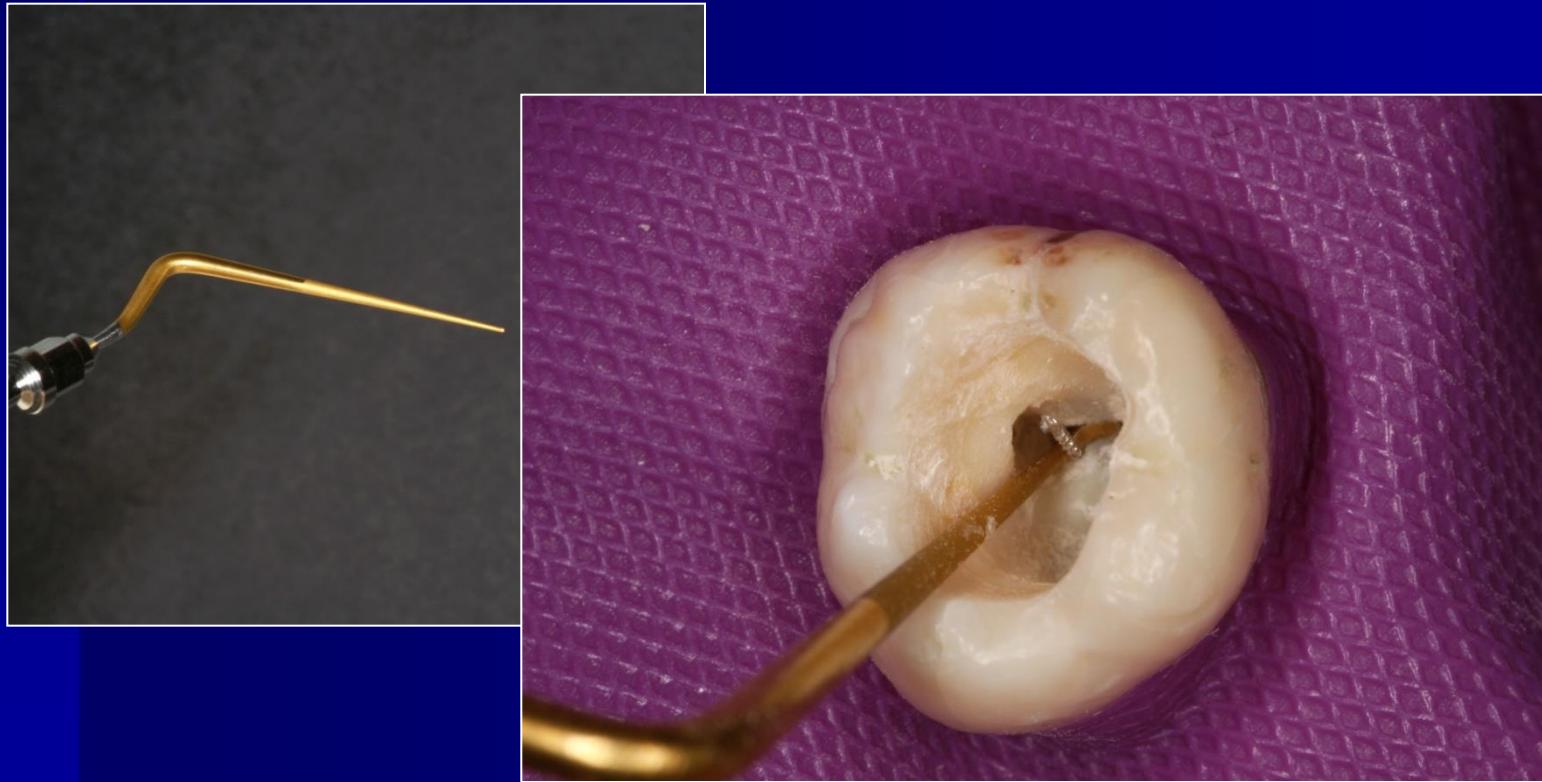

Apical surgery



Endodontics

Root canal shaping
Activation of irrigation

