


MUNI

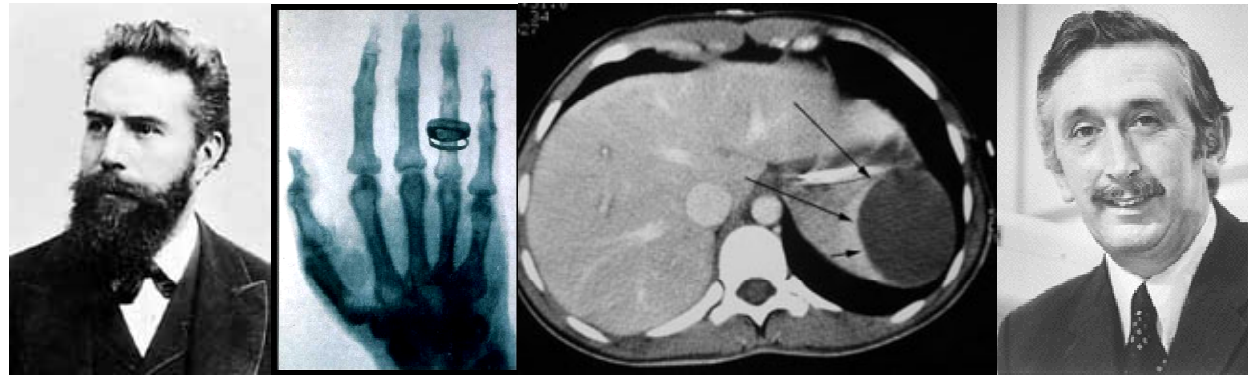

Wilhelm Conrad
Roentgen

1845 - 1923

Godfrey N.
Hounsfield

1919 - 2004

Lectures on Medical Biophysics

X-ray Imaging (XRI) and CT

X-Ray Imaging

- X-ray imaging (XRI) is still one of the most important diagnostic methods used in medicine. It provides mainly morphological (anatomical) information - but may also provide some physiological (functional) information.
- **Its physical basis is the different attenuation of X-rays in different body tissues.**
- We have to keep in mind that X-rays may lead to serious health effects (e.g., cancer) for both patients and healthcare professionals (HCP). Thus, strict legal radiation protection safety measures exist to avoid any unnecessary harm to both patients and the HCP. We will deal with them in a special lecture.

Content of the Lecture


- Projection XRI devices
- Image formation
- Projection X-ray devices for special purposes
- CT
- Radiation dose and health risk

Projection XRI Devices



MUNI

X-Ray Production – Low Power X-Ray Tube used in Dental Units

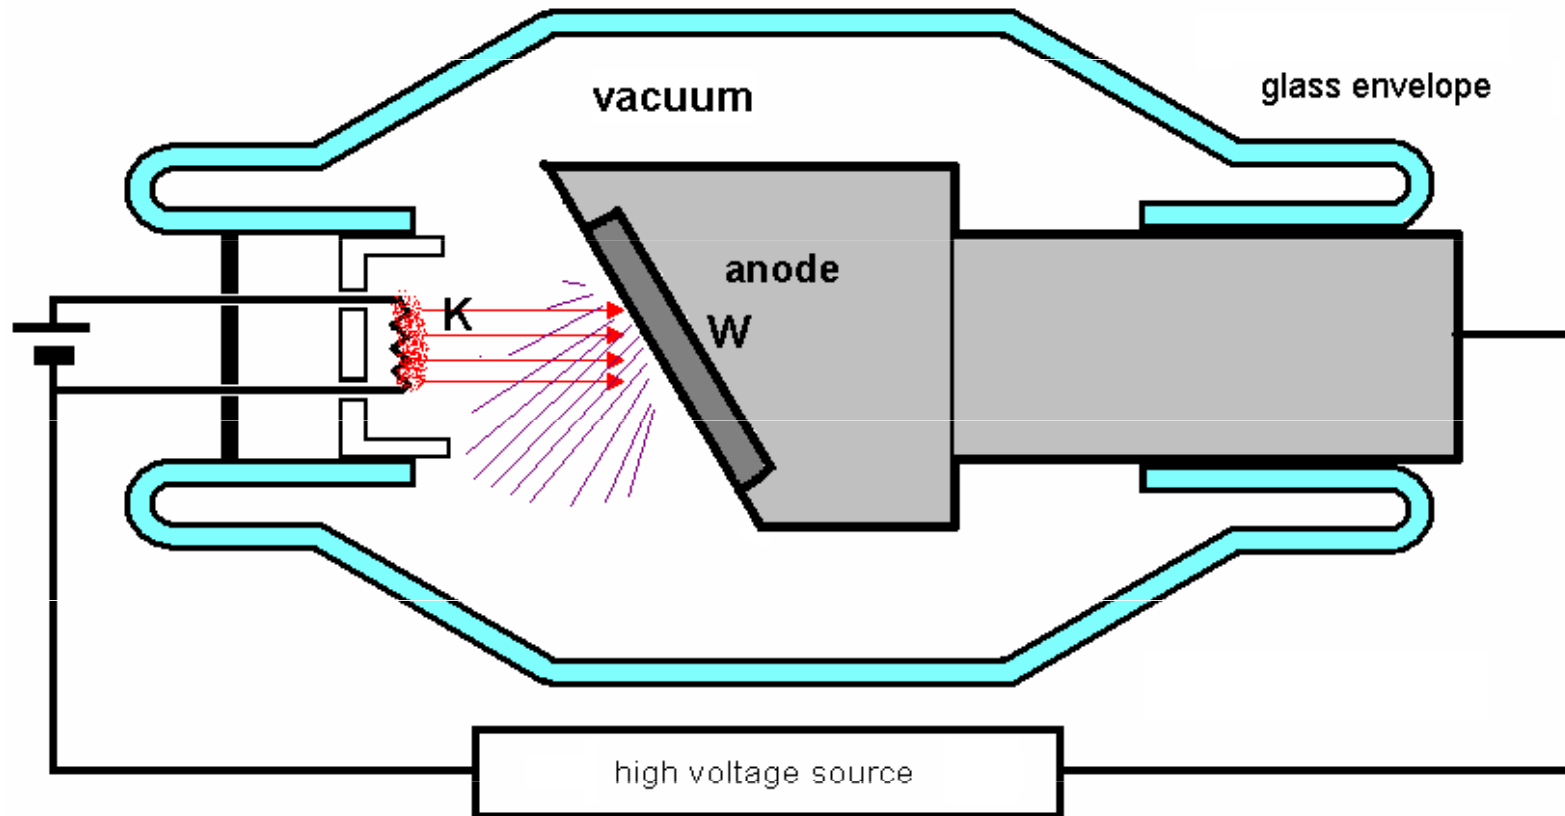

Scheme of an X-ray tube. K – hot filament cathode, W – tungsten plate.

High-Power Rotating Anode Tube



Production of X-rays

➤ An electron with an electric charge e ($1.602 \cdot 10^{-19}$ C) in an electrostatic field with potential difference U (voltage, in this case it is the voltage across the anode and the cathode) has **potential energy**

E_p :

$$E_p = U \cdot e$$

➤ In the moment just before impact of the electron onto the anode, its potential energy E_p is fully transformed into its **kinetic energy** E_K .

Thus:

$$E_p = E_K = U \cdot e = \frac{1}{2} m \cdot v^2$$

➤ On impact, the E_K is transformed into x-ray photon energy (less than 1%) and heat energy (99%). This heat can damage the tube.


Photon Energy and Tube Voltage

- If ALL the kinetic energy of the accelerated electron is transformed into a SINGLE X-ray photon, this photon will have energy:

$$E = h \cdot f = U \cdot e$$

- This is the maximum energy of the emitted photons. It is directly proportional to the voltage U across the anode and cathode. h is the Planck constant.
- Hence if we want to increase the energy of the photons all we have to do is increase the voltage!
- The higher the energy of the photons the less they are attenuated by the body - the higher the penetration. This is important when imaging thick body parts or fat patients!

Photon Energy Histogram

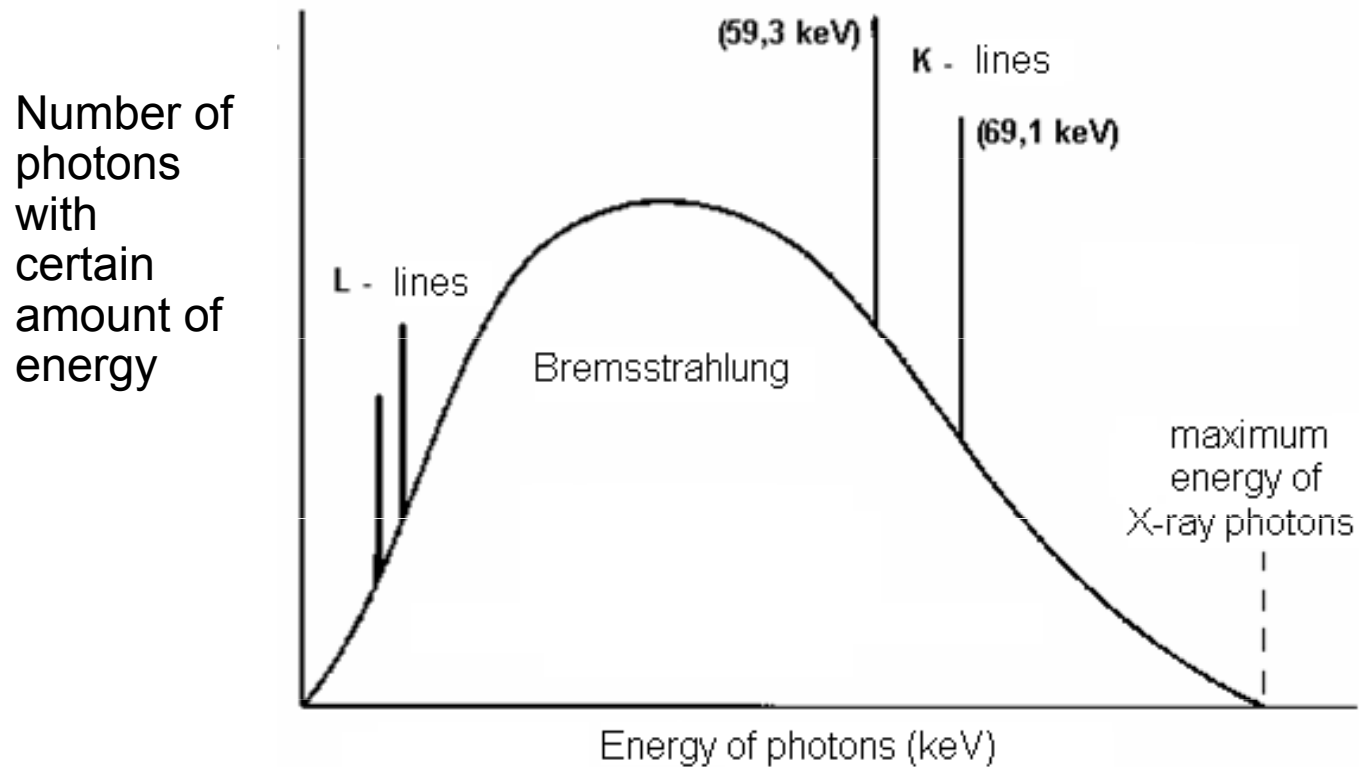

Main Parts of the XRI Device

- **X-ray tube**
- **Voltage-Current Generator:**
 - **High Voltage Transformer** – supplies high voltage (up to 150kV)
 - **Rectifier** - produces unidirectional tube electron current
 - **When increasing the magnitude of the electron beam current** (by changing the cathode heating) **the photon fluence rate** (i.e. number of photons per unit area per second) **of the X-ray beam increases** - however the energy of individual photons does not.
 - The energy of the individual photons can be increased by increasing the voltage between the anode and cathode.
- **Control panel** – today most parameters of the device (including voltage and current) are controlled by means of a computer. It is located outside the examination room or behind a shield made of glass containing lead (to protect the radiological assistant).
- Main **mechanical parts**: tube stand, examination table, grid for removing scattered photons ('Bucky'),
- **X-ray detector**: cassette with radiographic film and adjacent fluorescent screens (**in radiography**) or image intensifier (both on the way out) or **flat panel digital detector** (**in fluoroscopy or in general**).

Passage of X-rays through Patient's Body

- X-rays emitted from a small **focal area** of the anode propagate in all directions. In the tube envelope, some low energy photons are absorbed. Further absorption of these photons occurs in the **primary filter**, made of aluminium sheet. It absorbs low energy photons which would be absorbed by surface tissues and do not contribute to the image formation (unnecessary patient dose). X-ray beam is delimited by rectangular **collimator plates** made of lead.
- The rays then pass through the body where transmission or absorption or scattering may occur. After that they pass through the **grid**, which is in front of the detector to remove scattered photons as these would degrade the image.

Image Formation

- X-ray image is an analogy of a 'shadow' cast by a semitransparent and structured body illuminated by light beam coming from an almost point source. The image is formed due to different **attenuation** of the beam by the different body tissues and by projection of the structures on a film or an electronic X-ray detector.
- The image can be visualised by means of
 - **Radiographic film / screen** and subsequent development
 - **Digital plate** and displaying image on a PC monitor
 - **Image intensifier** and digital CCD camera connected to a monitor

Attenuation of Radiation

A beam of X-rays (any radiation) passes through a substance:

absorption + scattering = attenuation

A small decrease of radiation intensity $-dI$ in a thin substance layer is proportional to its thickness dx , intensity I of radiation falling on the layer, and a specific constant μ :

$$-dI = I \cdot dx \cdot \mu$$

After rewriting:

$$dI/I = -dx \cdot \mu$$

After integration:

$$I = I_0 e^{-\mu x}$$


I is intensity of radiation passed through the layer of thickness x , I_0 is the intensity of incoming radiation, μ is **linear coefficient of attenuation** [m^{-1}] depending on kind of radiation, medium and its density.

The **mass attenuation coefficient** μ/ρ does not depend on the density.


The symbol „d“ comes from differential calculus, we can imagine it as a very small change.

Cassettes for Radiographic Films

FLUORESCENT
screens reduce
dose of radiation
about 50-times

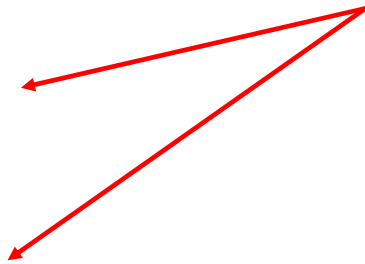

Digital Imaging Plates

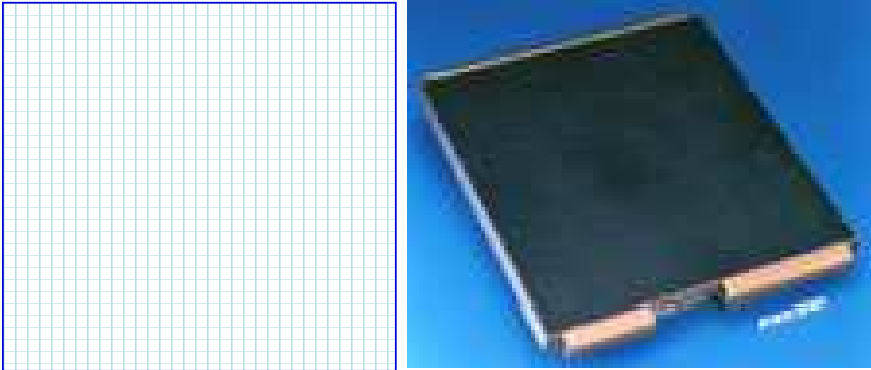

Imaging plate consists of an array of very small sensors



„bucky“ – see slide 24

Matrix of amorphous silicon (aSi) photodiode light sensors

Phosphorescent layer of CsI (necessary for patient dose reduction as aSi is not good absorber of X-rays)


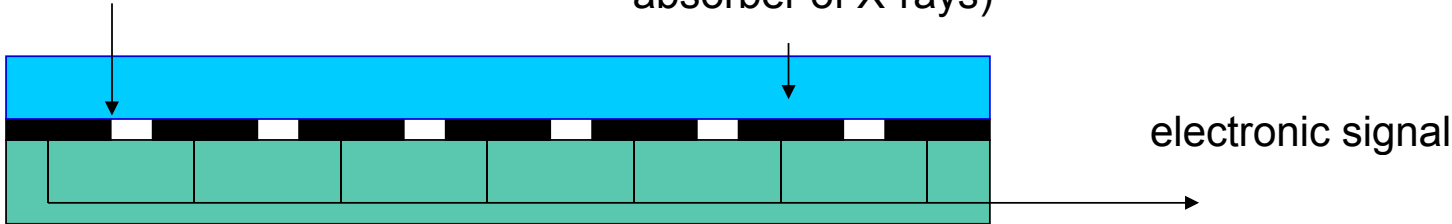


Image Intensifier

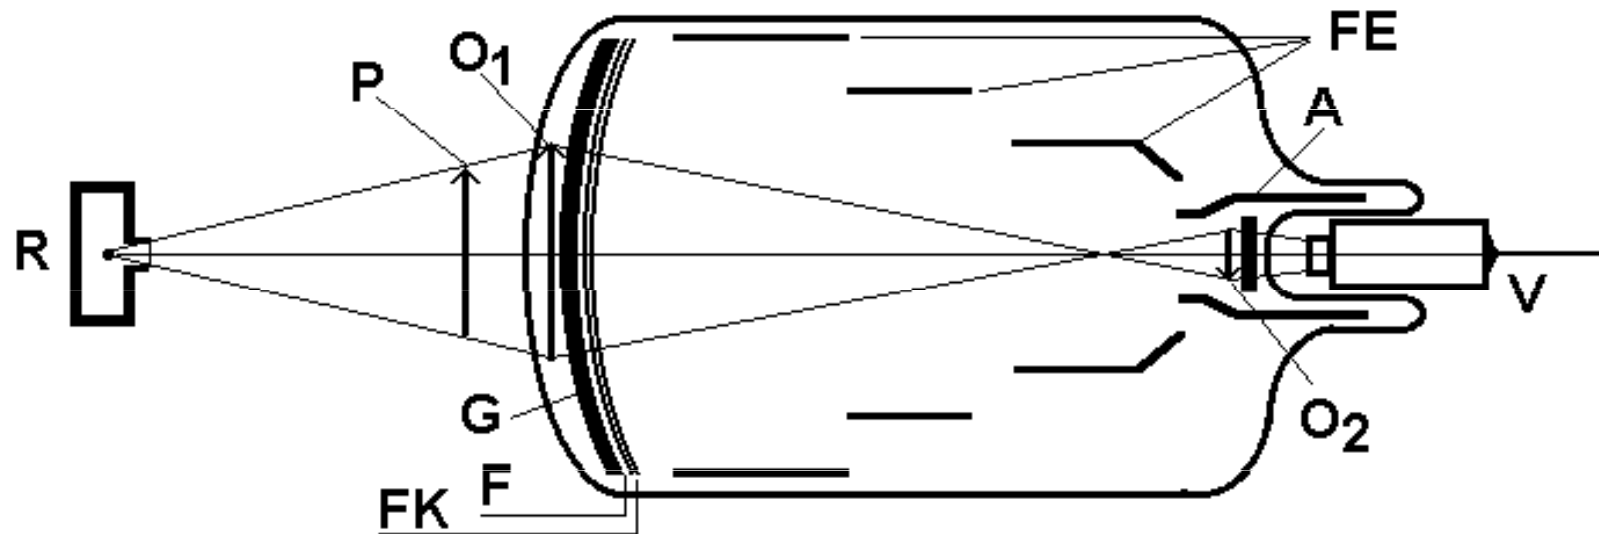

R – X-ray tube, P - patient, O₁ – primary picture on a fluorescent screen, G – glass carrier, F – fluorescent screen, FK - photocathode, FE – focussing electrodes (electron optics), A - anode, O₂ – secondary image on the anodic screen, V – video-camera. Individual parts are not proportionally depicted.

Different Ways how to Obtain DIGITAL Images

(mammographic systems)

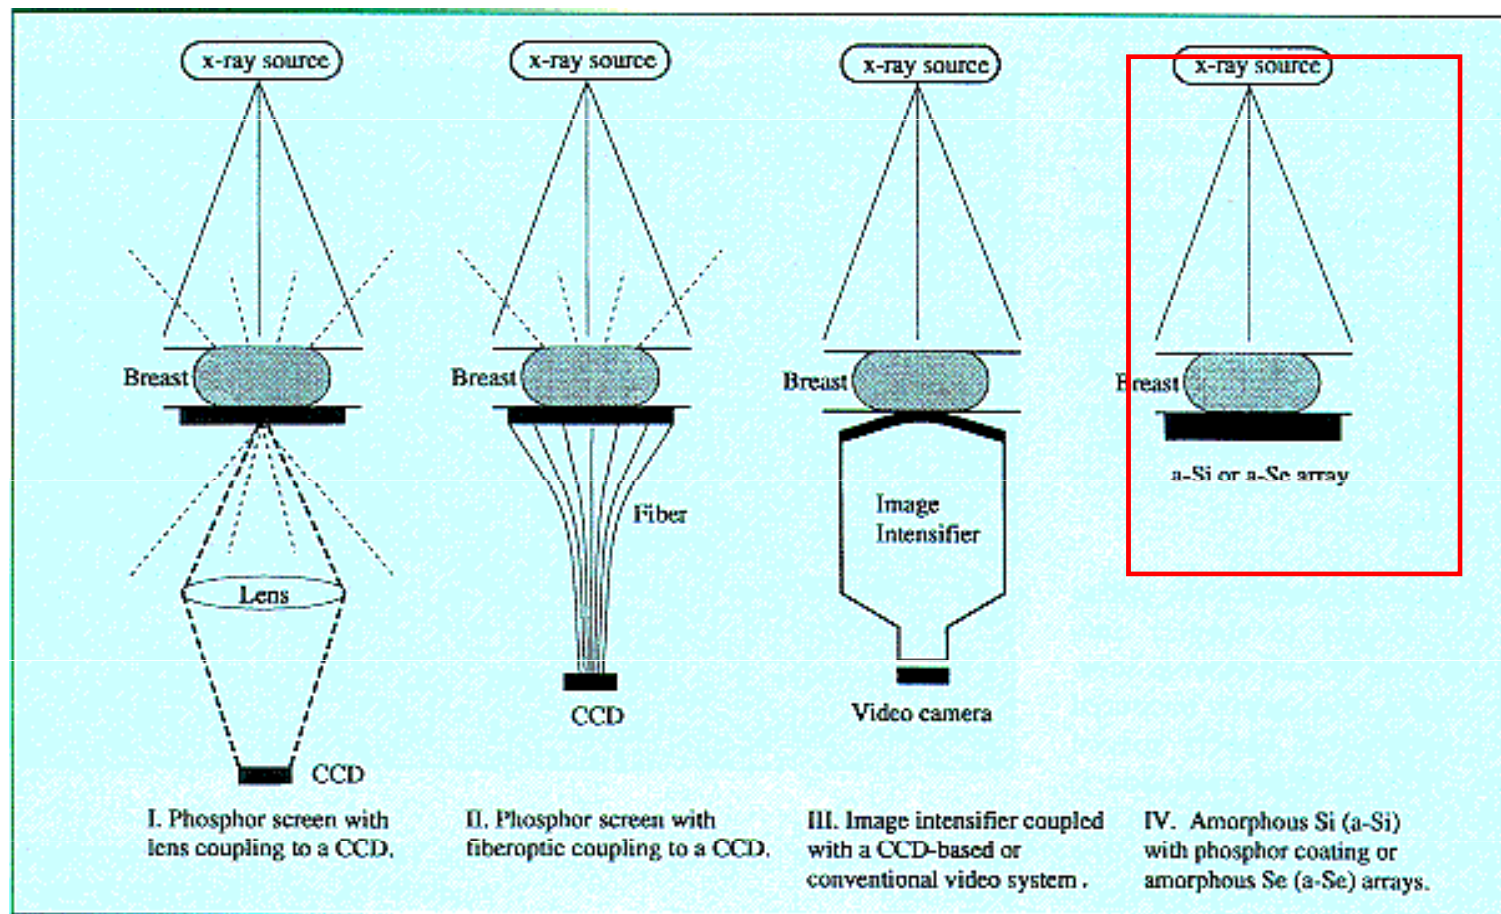


Fig 1. – Schematic diagram of solid-state x-ray detector technologies employed in the development of digital mammography systems. The small-dashed lines in systems I and II represent the losses due to the phosphor glow emitted in all directions.

<http://www.moffitt.org/moffittapps/ccj/v5n1/department7.html>


MUNI

Blurring of the Image

No radiograph (an X-ray image) is absolutely sharp. Boundaries between tissues are depicted as a gradual change of gray scale. This non-sharpness (blurring) has several reasons:

- 1) **Movement blur** – accidental, breathing, pulse waves, heart action etc. They can be reduced by shorter exposure times with more intense X-ray radiation.
- 2) **Geometric blur** is caused by finite focal area (focus is not a point). The rays fall on the boundary of differently absorbing media under different angles – blurring of their contours appears
- 3) The light emitted by fluorescent screens attached to the film or digital detector does not only illuminate the corresponding part of the film or detector, but also spreads out to surrounding areas.

Geometric Blur ('penumbra')

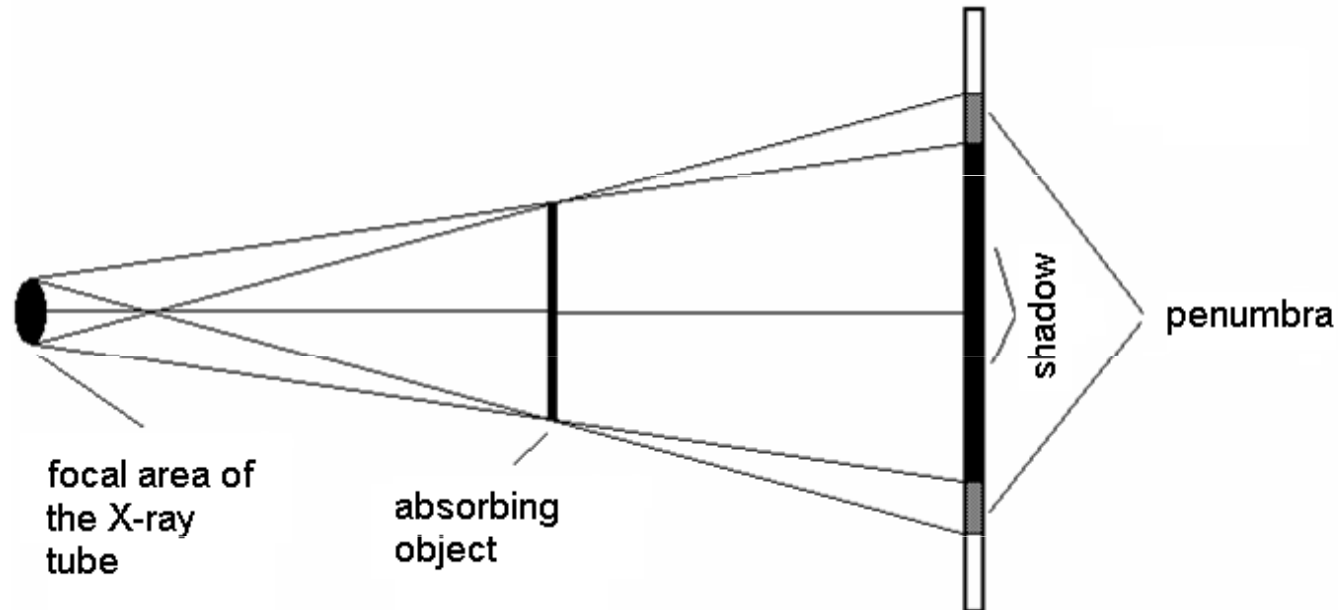

Geometric penumbra can be **reduced** by:

- Choosing a small focal spot size (but it increases risk of damage to tube anode by heating)
- Decreasing the distance between the patient and the detector
- Increasing the distance between the X-ray tube and the patient

Interactions of X-ray Photons with Matter: ABSORPTION by Photoelectric Effect (PE)


- Photon disappears ('is absorbed') after hitting an atom and an electron is ejected from electron shell of the atom (typically K-shell). Part of the photon energy $h \cdot f$ is necessary for ionisation. Remaining part of the photon energy changes into **kinetic energy** ($1/2m \cdot v^2$) of the ejected electron. The electron knocks electrons out of atoms of the body and produces ionization of these atoms. The **Einstein equation for photoelectric effect** holds:

$$h \cdot f = E_b + 1/2m \cdot v^2,$$

E_b is binding (ionisation) energy of the electron (called also **work function**).

- The probability for PE increases with proton number and decreases with increasing photon energy (this is why lead is used for shielding and why higher energy beams are more penetrating).

Photoelectric Effect

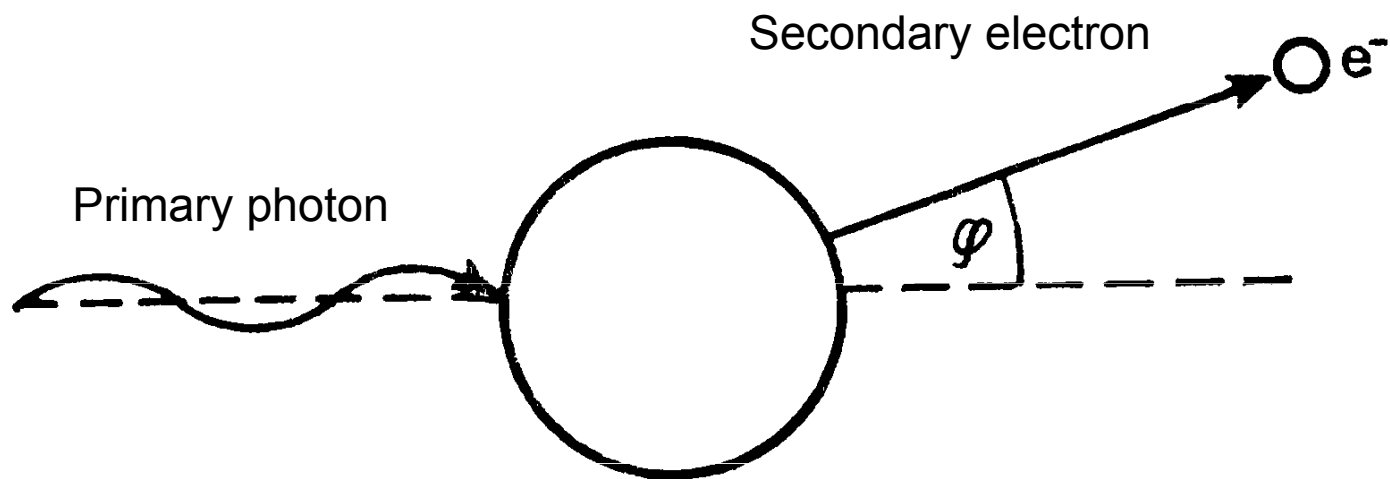


Interactions of X-ray Photons with Matter: Compton Scatter (CS)

- At higher energies of photons, the photon energy is not fully absorbed – **a photon of lower energy appears**. The binding energy of the electron E_b is negligible in comparison with the photon energy. We can write:


$$h \cdot f_1 = (E_b) + h \cdot f_2 + 1/2m \cdot v^2,$$

- where f_1 is frequency of incident photon and f_2 is frequency of the scattered photon.
- CS is more probable than PE for primary photon energies 0.5 - 5 MeV and does not depend on the the proton number of interacting atom which explains why images at such energies would be practically useless.

Compton Scatter

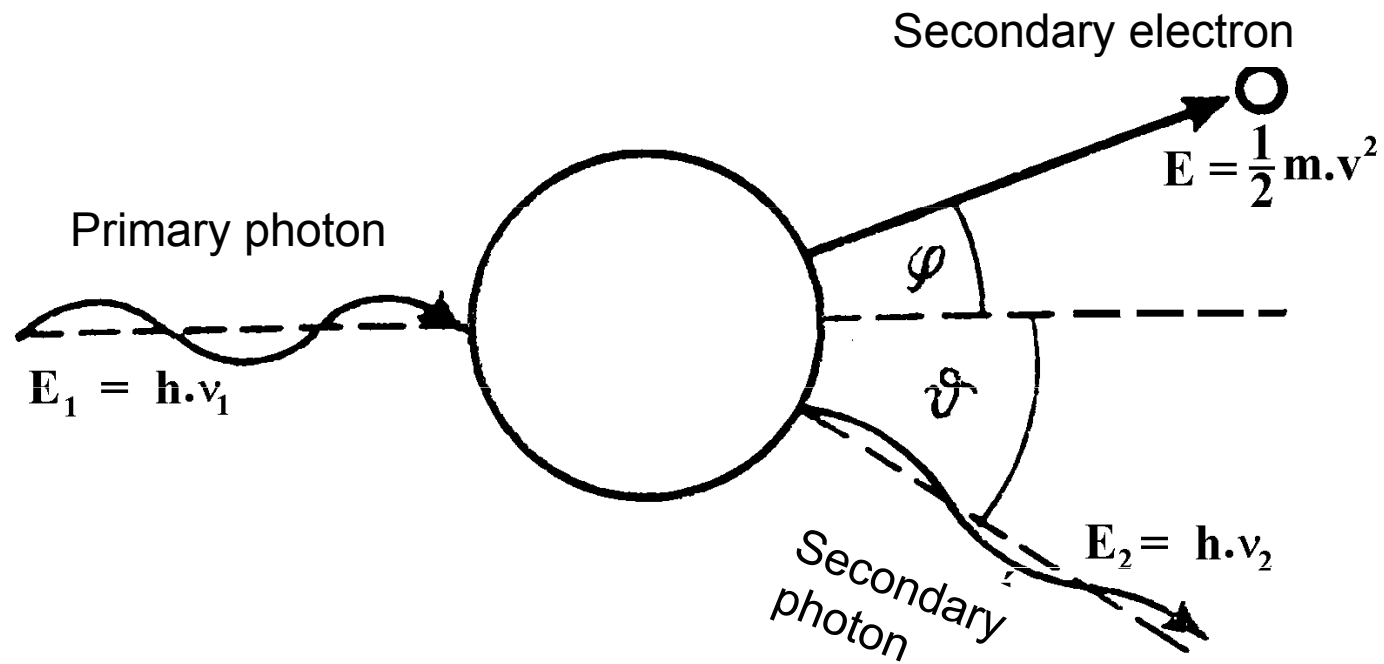

Principle of the Bucky Grid

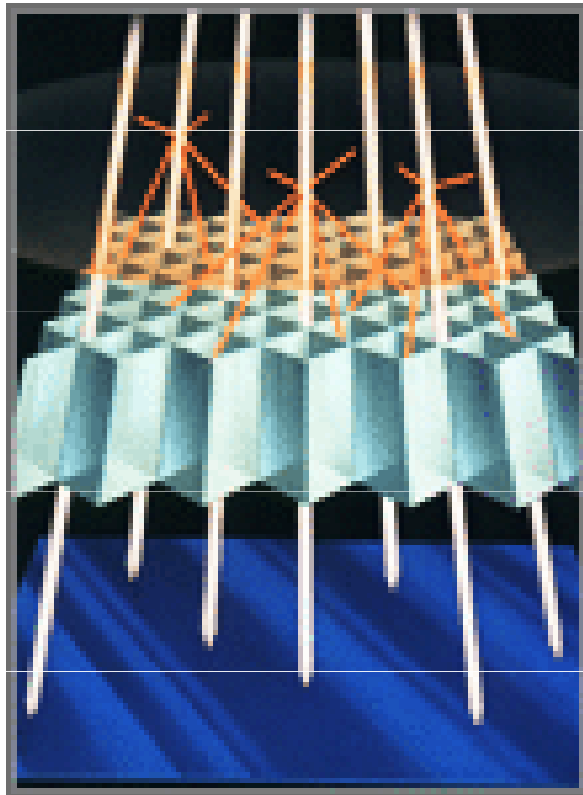

<http://www.cwm.co.kr/pro213.htm>

The Bucky grid stops a substantial part of the scattered rays whilst allowing the useful photons to pass through. However unfortunately grids also absorb part of the useful radiation. Hence a higher amount of x-rays must be used to produce a good image – this increases the dose of radiation to the patient. Hence for example grids are not used with thin children as the level of scatter is low anyway.

Use of the Contrast Agents

- The soft tissues only slightly differ in their attenuation. Therefore they cannot be distinguished in a common radiograph. That is the reason for the use of pharmaceuticals called **contrast agents**.
- The attenuation of certain tissues can be increased or lowered. **Positive contrast** is achieved by substances having a high proton number as the probability of the photoelectric effect is increased. A suspension of **barium sulphate**, “barium meal”, is used for imaging and functional examination of GIT. In examinations of blood, biliary and urinary vessels etc. **compounds with high content of iodine** are used.
- Hollow inner body organs can be visualised by **negative contrast**. Air or better CO₂ can be used. The cavities are filled by gas, inflated, so that they can be visualised as structures of very low attenuation (pleural space, peritoneum, brain chambers in the past).

Positive and Negative Contrast



Contrast image of the appendix – diverticulosis – combination with negative contrast

<http://www.uhrad.com/ctarc/ct199b2.jpg>



Horseshoe kidney – positive contrast – we can see renal pelvis, calyces and also urethers

<http://www.uhrad.com/ctarc/ct215a2.jpg>




Pneumoencephalograph – negative contrast of brain chambers – history of medicine

<http://anatomy.ym.edu.tw/Nevac/class/neuroanatomy/slide/k42.jpg>

Devices for Special Uses - Examples

- Dental X-ray devices
- Mammographic devices
- Angiography (image subtraction systems, formerly image intensifier based; now increasingly digital detector based)

X-ray Devices in Dentistry

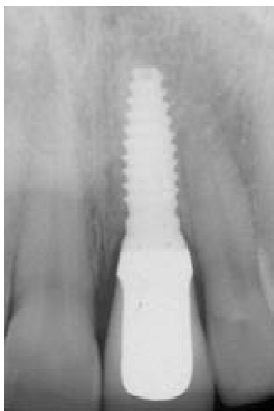

<http://www.gendexray.com/765dc.htm>

X-ray image of a dental implant

Panoramic screening – orthopantomography

very useful in e.g. orthodontics


<http://www.gendexray.com/orthoralix-9000.htm>

Mammography



Mammography is the process of using low-dose X-rays (usually around 0.7 mSv) to examine the female breast. It is used to look for different types of tumours and cysts. In some countries routine (annual to five-yearly) mammography of older women is encouraged as a screening method to diagnose early breast cancer. It is normal to use low energy (soft) X-rays (molybdenum anode).

Digital Subtraction Angiography

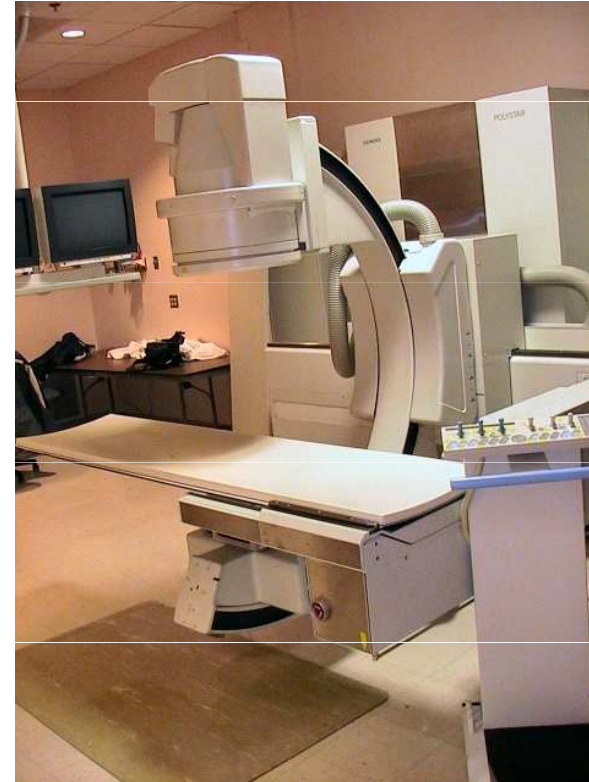

http://zoot.radiology.wisc.edu/~block/Med_Gallery/ia_dsa.html

MUNI

Computerised Tomography - CT

- The first patient was examined by this method in London, 1971.
- The apparatus was invented by English physicist Hounsfield, (together with American Cormack, Nobel award for medicine, 1979)



Principle of CT

- Principle: The CT scanner is a complex instrument for measuring the X-rays attenuation in individual voxels (volume analogies of pixels) in narrow slices of tissues.
- Method of measurement: A narrow fan-beam of X-rays is passed through the body and the emerging radiation measured by an arc of detectors. This is repeated at different angles till enough information is available to be able to calculate the attenuation coefficient in the patient voxels. A „map“ of attenuation is calculated – a tomogram.

Examples of CT Scans


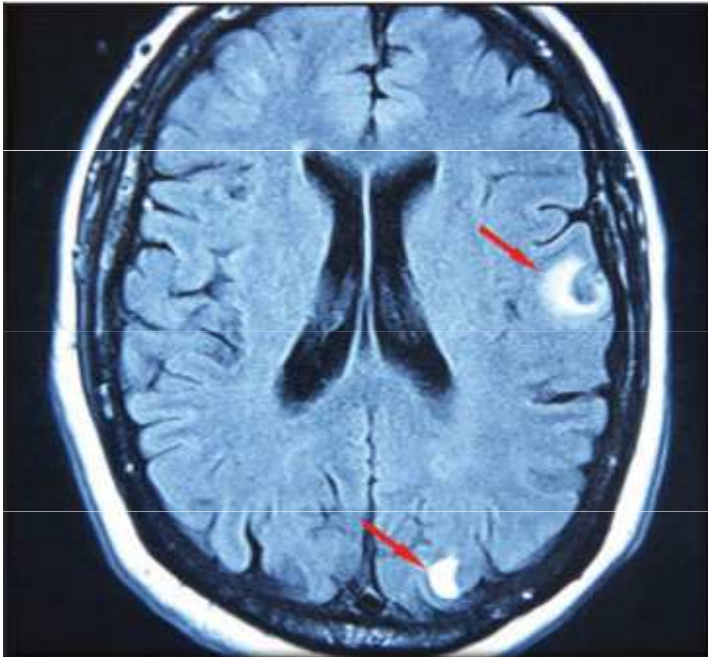


Figure 2. Brain CT scan with multiple melanoma metastases in a patient who presented with leg pain only

Metastatic lesions in brain

<http://www.mc.vanderbilt.edu/vumcdept/emergency/mayxr3.html>

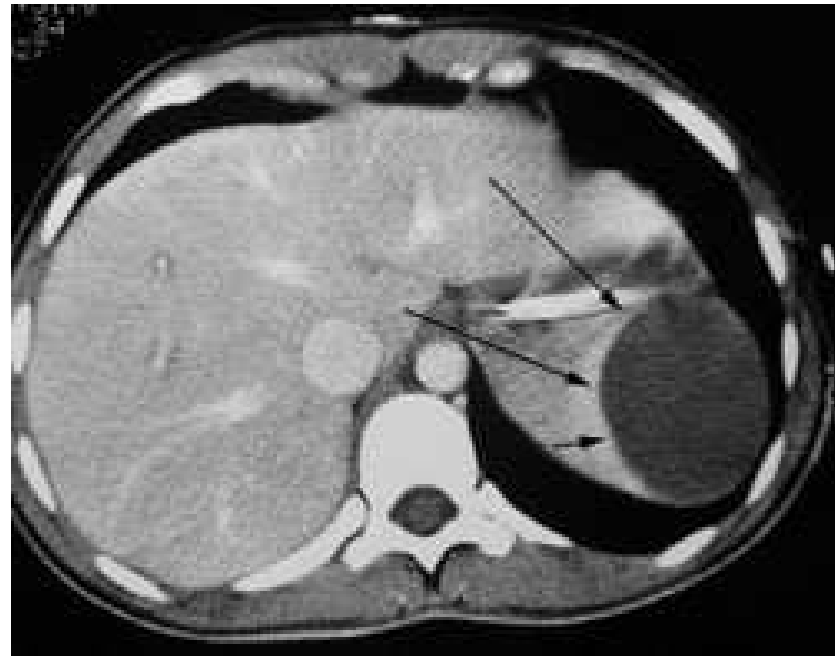


Extensive subcapsular haematoma of spleen in patient after car accident

<http://www.mc.vanderbilt.edu/vumcdept/emergency/apr7xr1a.html>


Advantages of CT over Projection XRI

- Much higher contrast than projection XRI - 0.5% difference in attenuation can be resolved because:
 - Almost total elimination of effects of scatter
 - X-ray measurements are taken from many angles
- Thus, we can see and examine different soft tissues.
- No overlapping of anatomical structures
- Less distortion as measurements are taken from many angles


Four Generations of CT

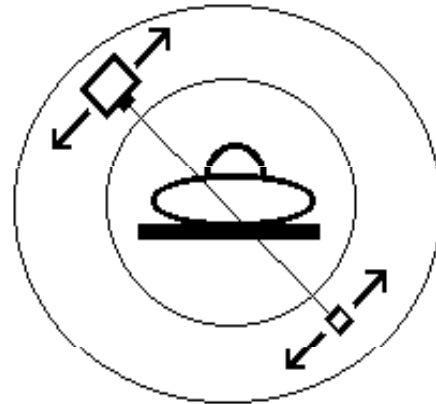


1. Generation

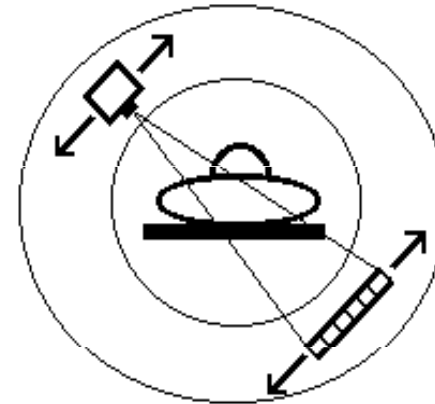

2. Generation

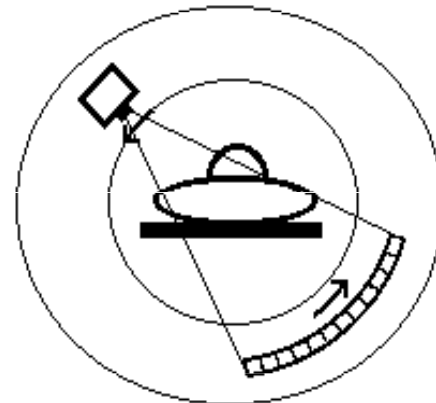


3. Generation

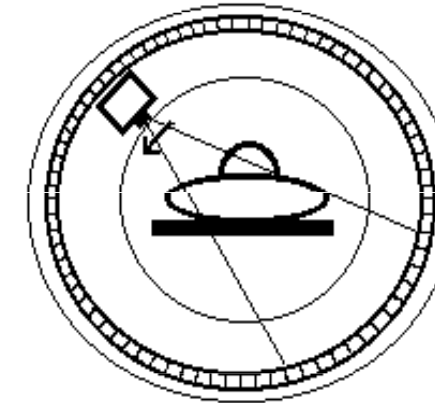


4. Generation

Principle of Spiral (3D) CT

X-ray tube and detectors revolve around the shifting patient

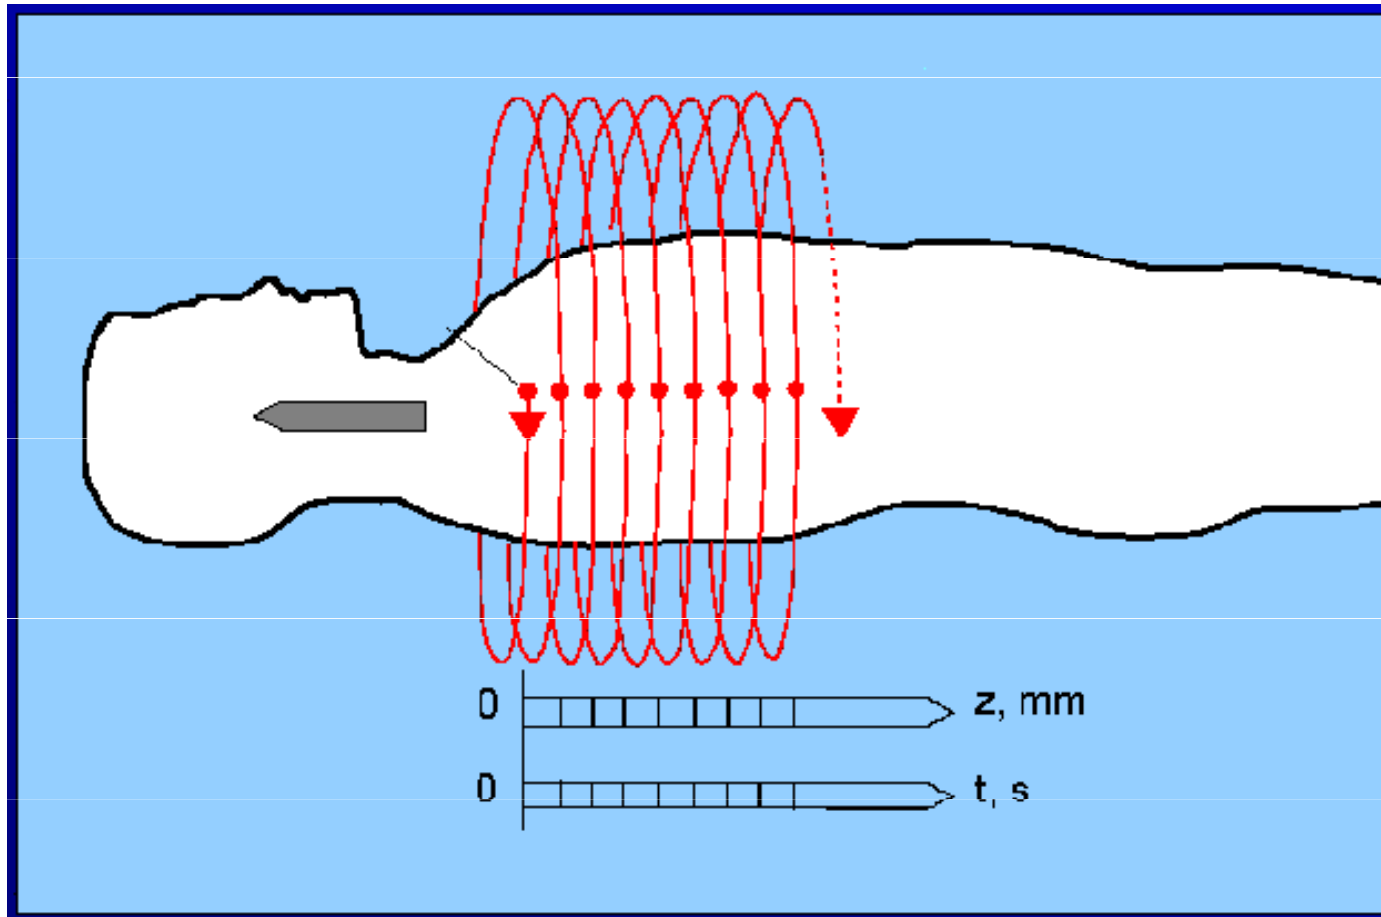

Multislice CT and Cone beam CT

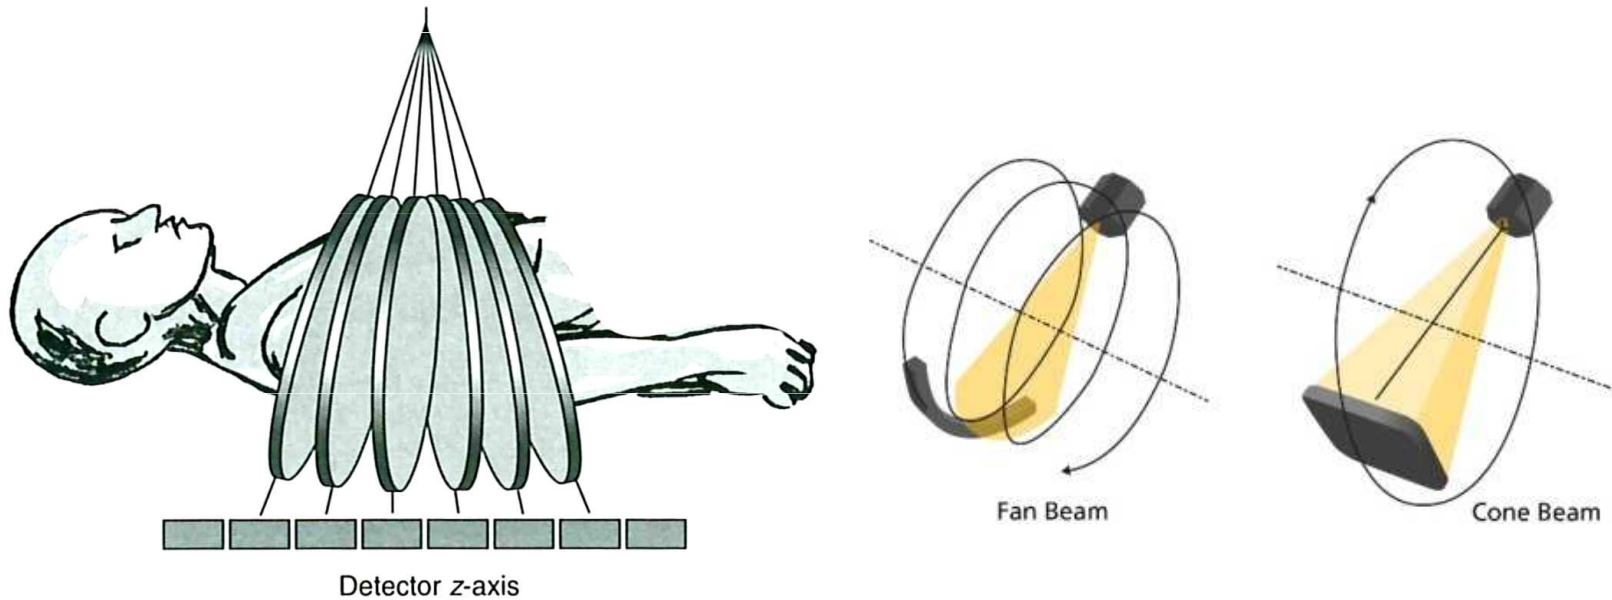

Fast 3D reconstruction is possible

Hounsfield (CT) Units

In order to simplify calculations we use Hounsfield Scale units (HU) for amount of attenuation.

On this simplified scale water is 0 HU, air is -1000 HU, compact bone is about +1000 HU.

A scale of 2000 HU is available for CT examination of body tissues. In most cases, it is senseless to attribute them to all of the grey scale levels (our eye is able to distinguish only about 250 levels of grey). Most of the soft tissue HU values range from 0 to +100. Thus we use only limited „diagnostic window“ of these units in practice, e.g. from -100 to +100.


$$HU = \frac{\mu_T - \mu_W}{\mu_W} \cdot k$$

W – water


T – tissue

$k = 1000$

„Diagnostic Window“ of HU

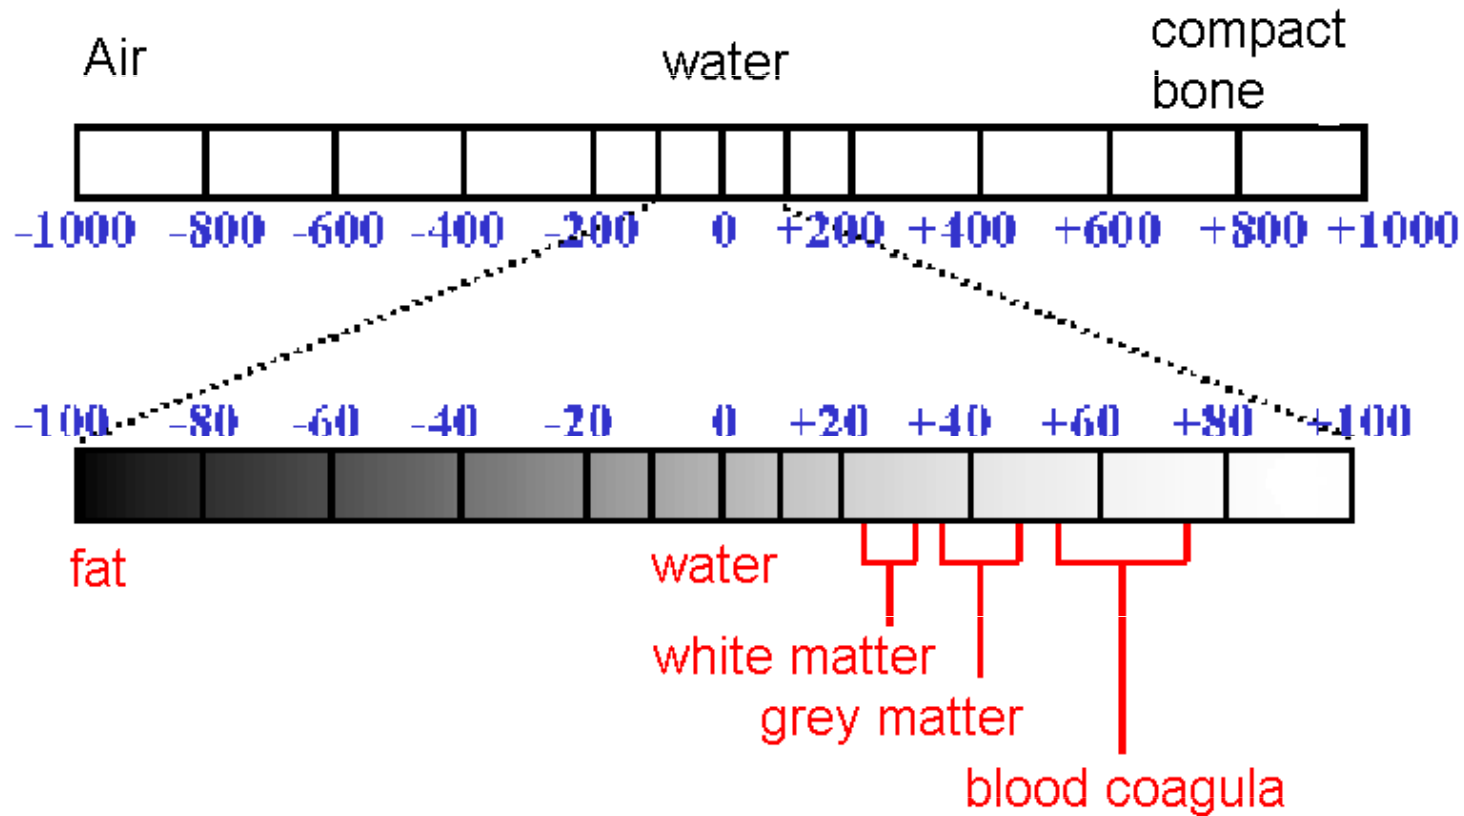

3D CT - Color Coding

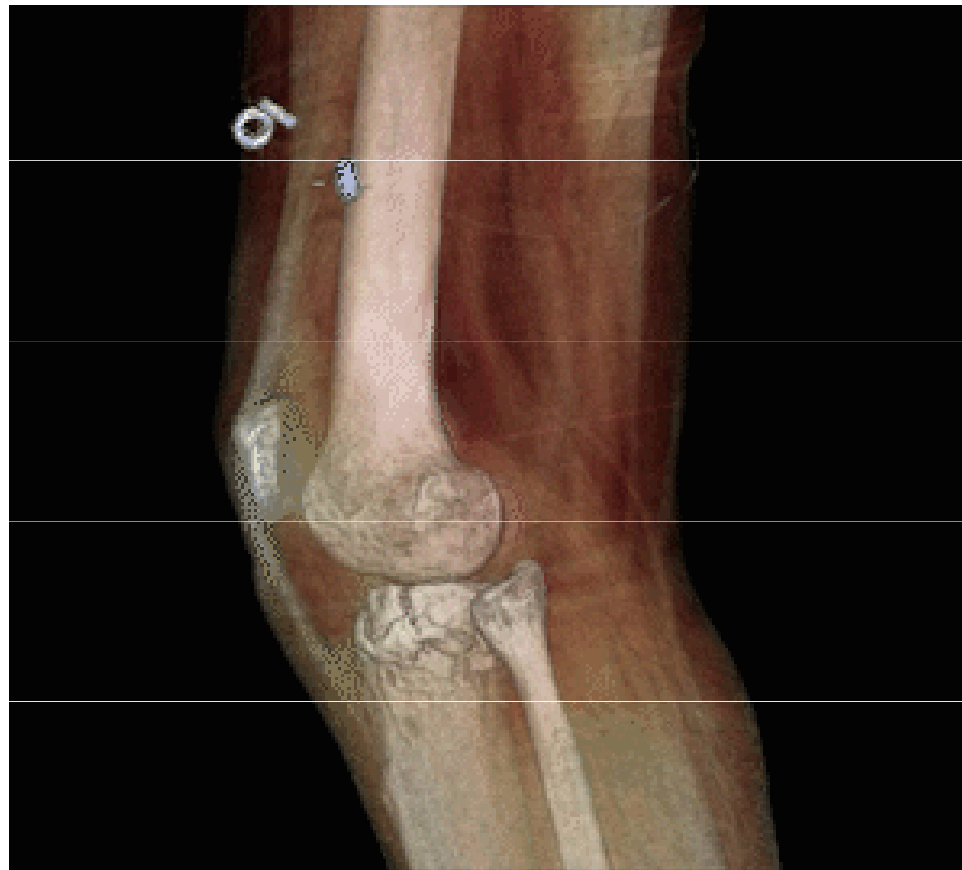

<https://www.carestream.com/en/us/medical/products/carestream-onsight-3d-extremity-system>

M U N I

Some Typical Doses


- From natural sources: 2 mSv per year
- Chest X-ray: <1 mSv
- Fluoroscopy: 5 mSv
- CT Scan: 10 mSv
- Medical doses are increasing with 'better be safe than sorry' medicine and the ease of use of modern imaging devices (e.g., spiral CT compared to conventional CT).

M U N I

Appendix: Dental Radiography Devices



Direct Digital Dental Radiography

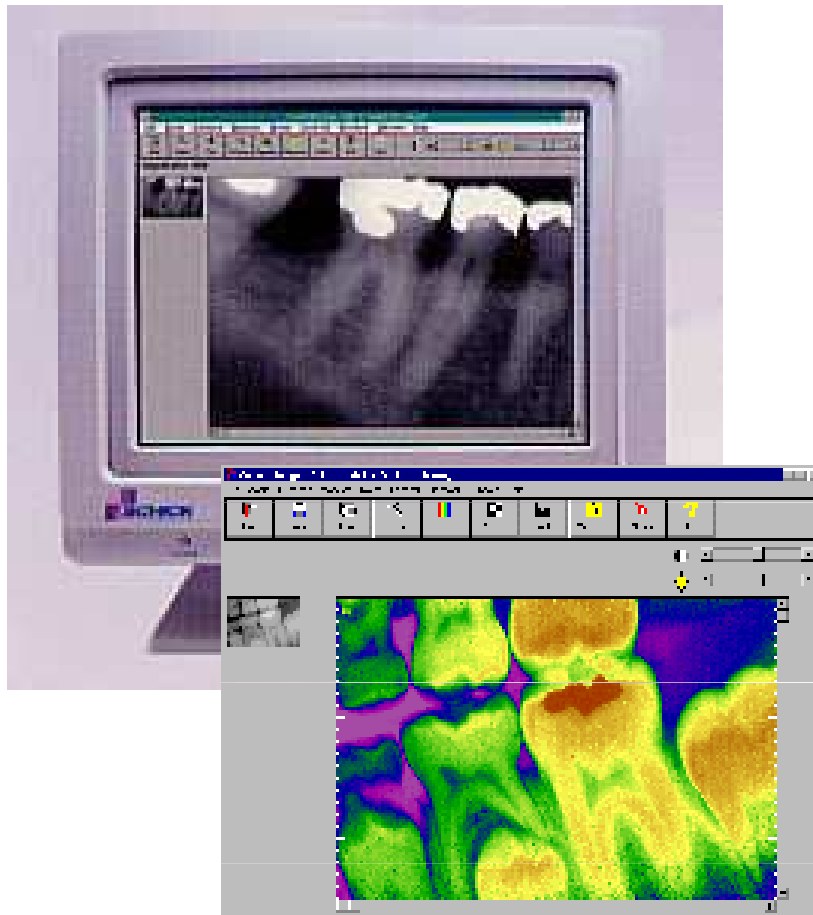


Sensor consists of photodiode matrix covered with a scintillator layer. Wireless sensors now available (using bluetooth or wifi).

Intra-Oral Image



Orthopantomographic (OPG) Unit

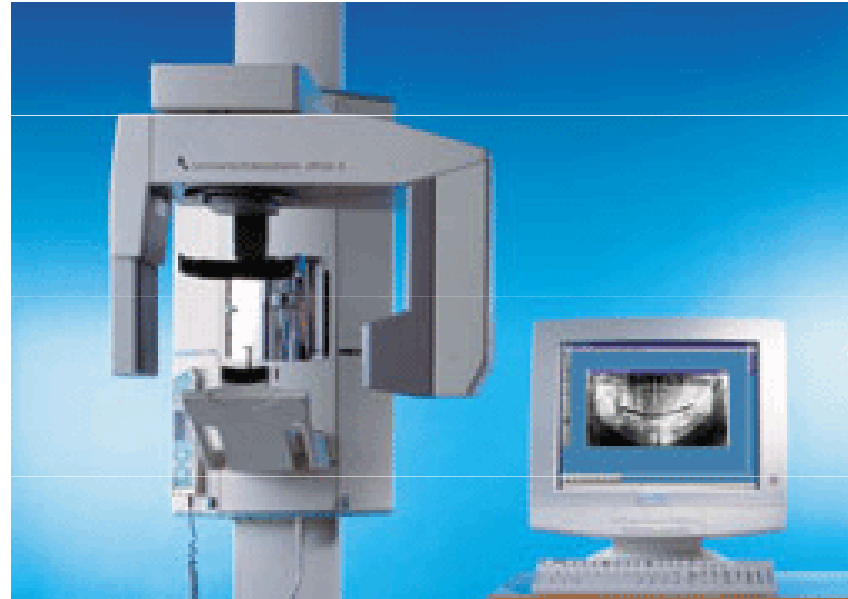

MUNI

Orthopantomographic (OPG) Image




You can see the so-called braces here. Used in orthodontics.

M U N I

Extraoral Cephalometric Image



Important for assessment of
e.g. cranium development
and before some orofacial
surgery!

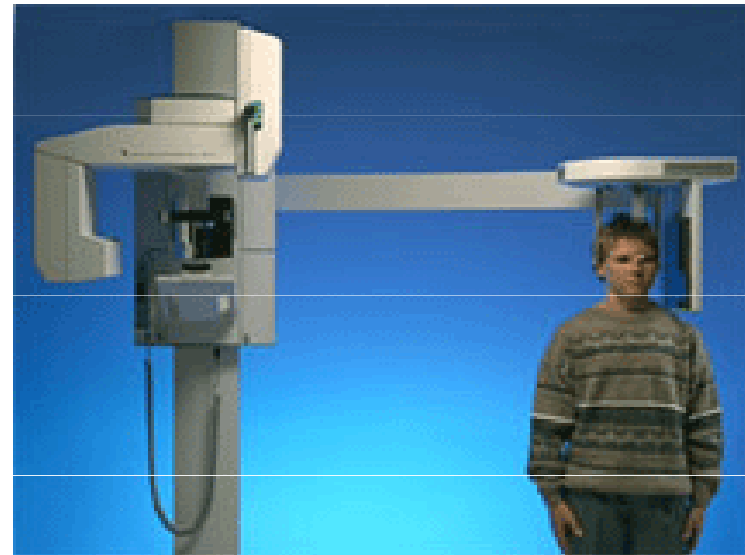

Radiation Protection Considerations

- Low individual dose but high collective dose technique, particularly since many young patients
- Protect eye and thyroid (sometimes latter close to or exposed to direct beam)
- As the dose, and therefore the risk to the developing fetus is so low there is no contraindication to radiography of women who are or may be pregnant providing that it is clinically justified. Very Good reference is:
 - RP136 European guidelines on radiation protection in dental radiology - The safe use of radiographs in dental practice. 2004. EU publication.

Dose Optimisation for Intraoral

- Devices
 - Constant power (CP) generator
 - filter: 1.5mm Al up to 70kV to reduce skin dose
 - Rectangular collimator recommended (if round-end collimator used, beam diameter <60mm at patient end of cone)
 - Digital devices need lower dose than film
- Protocol
 - use 60kV with CP generator
 - minimum SSD 200mm (cone should ensure this)
 - There is no need to use a lead protective apron (to protect gonads, except in rare cases) even in cases of pregnant patients. However in the case of pregnant patients, the use of a lead apron continues to be used in some states as it may reassure the patient
 - Some have suggested using thyroid collar for young patients (in CZ they use it even for adults)

Converting Round Collimators to Rectangular

The UK's Ionising Radiation (Medical Exposure) Regulations 2000 recommend the use of rectangular collimation to limit the radiation dose a patient receives during routine dental X-rays. DENTSPLY's Rinn Universal Collimator just clips onto any round-headed long-cone X-ray unit, converting it from round to the recommended rectangular collimation, in one easy step.



M U N I


Dose Optimisation in OPG

- Devices:
 - CP (constant power) generators
 - Automatic exposure control
 - Dead-man type switch
- Protocol:
 - Proper patient positioning and immobilisation to avoid repeats (e.g., in case of OPG chin rests on plastic support, head held by plastic earpieces, head surrounded by plastic guard)
 - Limit field size to area of interest
 - Thyroid collar inappropriate as it interferes with the beam in the case of OPG (note however often necessary in the case of cephalometry)



Authors:

Vojtěch Mornstein, Carmel J. Caruana



Content collaboration:

Ivo Hrazdira



Presentation design:

Lucie Mornsteinová



**Last revision September 2021, soundtrack added
September 2020**