


# ÚVOD DO KVANTITATIVNÍ REAL-TIME PCR

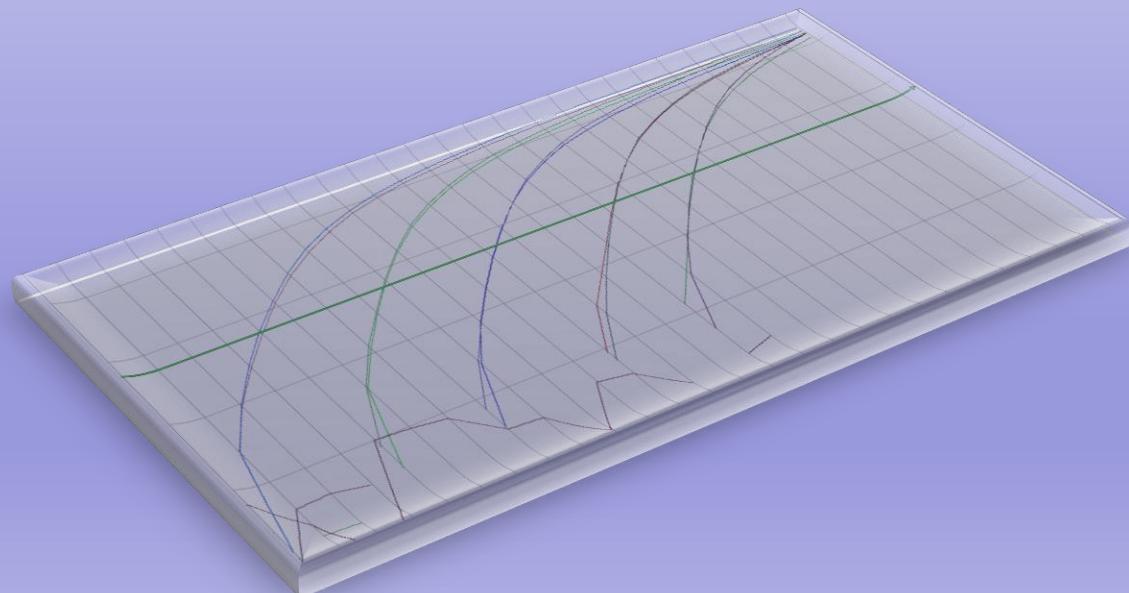

# Tipy na začátek

- Experimentální design
  - Co dělám?
  - Proč to dělám?
  - Jak to dělám?
- Kontrola všech chemikálií
  - Voda – alikvoty
  - Kit na RT – jen pro 1 studenta
  - Master mixy – omezené množství lidí

# Tipy na začátek

- Oddělení místností pre a post PCR
  - Izolace DNA, RNA
  - RT
  - PCR a post-PCR

# Tipy na začátek

- Negativní kontrola, pozitivní kontrola
- Příprava rozložení vzorků na destičce – no template control tak, aby nedošlo ke kontaminaci – co nejdále od vzorků s vysokou koncentrací
- Všechno rozmrazit na ledu, v temnu
- Reakční směs zhruba o 10% víc než je potřeba
- Destičku lze uchovat až 10 h v temnu a chladu
- Správně a úplně zlepit destičku fólií i na okrajích
- Alespoň duplikáty
- Po napipetování spin na centrifuze

# Kontroly

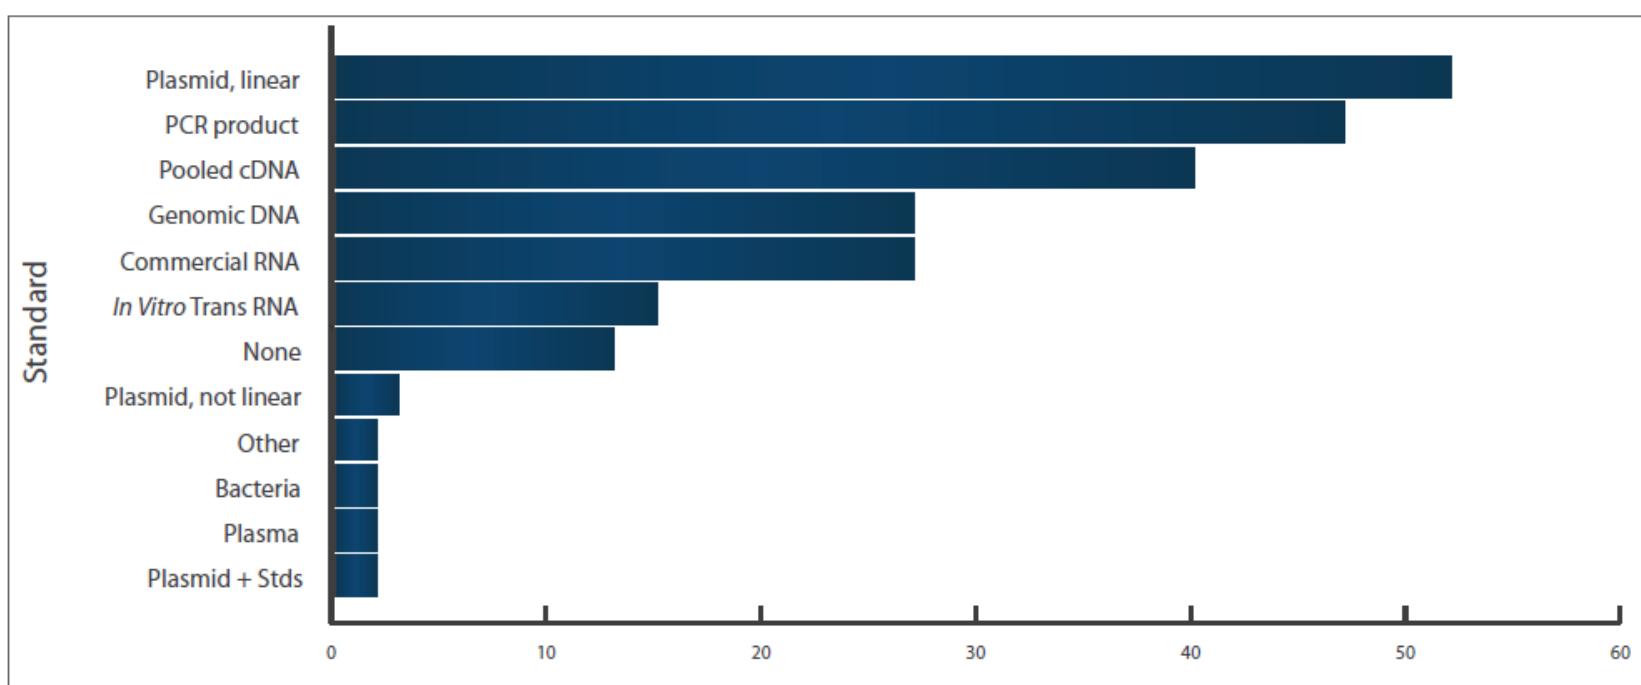


Figure 21: Most frequently used quantification standards. From Nucleic Acid Research Group, (NARG) survey 2007, <http://www.abrf.org/NARG/>

# Frekvence kontrol

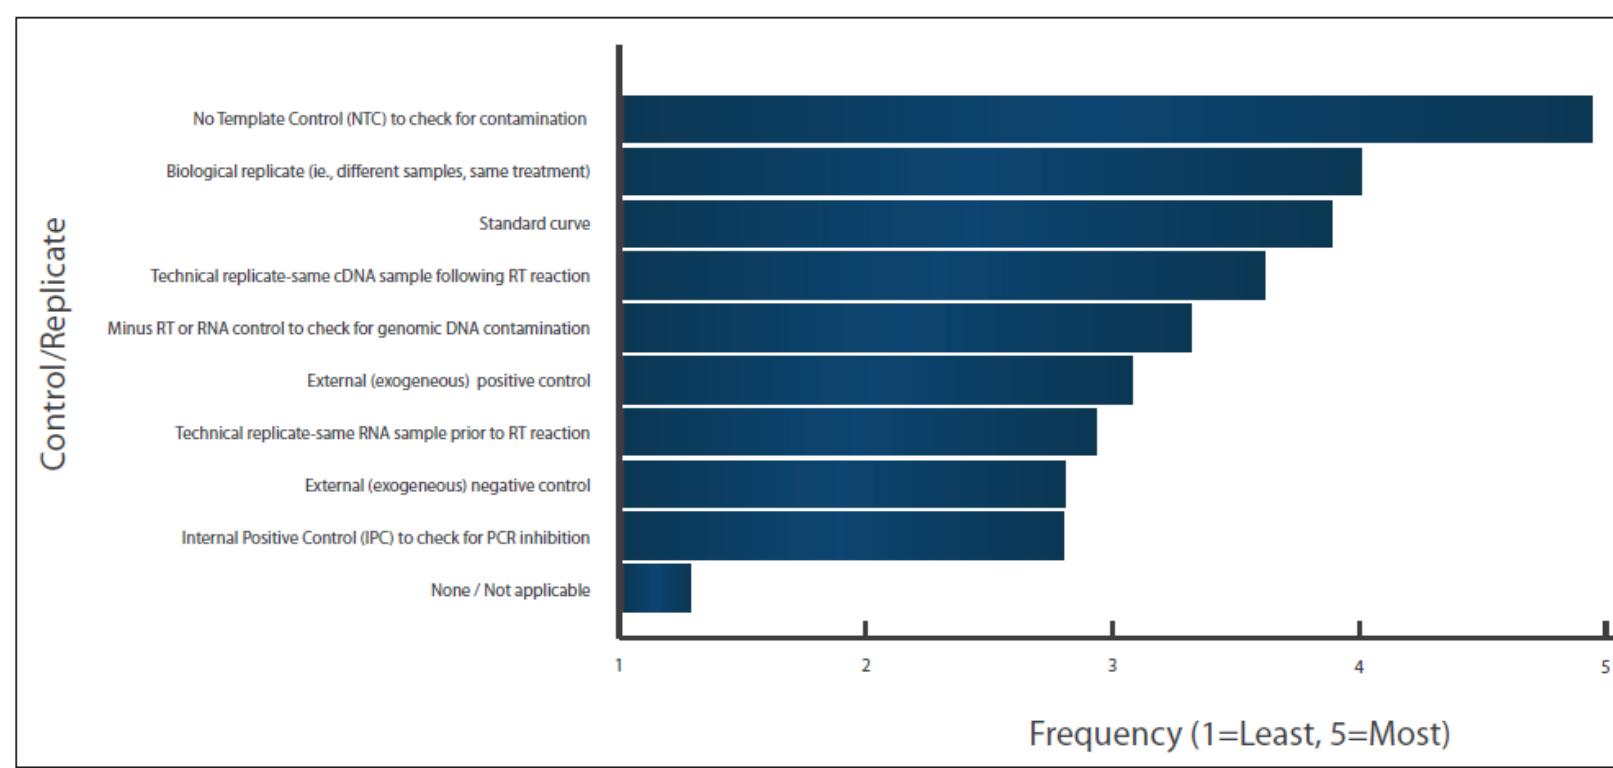


Figure 22: Frequency of replicates controls. From Nucleic Acid Research Group, NARG survey 2007, <http://www.abrf.org/NARG/>

# Negativní kontroly

- No RT- pokud ukáže amplifikaci - kontaminace genomovou DNA
- NTC - voda a reakční směs – žádný signál nebo alespoň o 8 cyklů později, 2 krát
- NAC - no amplification control, bez polymerázy

# Pozitivní kontroly

- Detekce kvality reagencií, přítomnost inhibitorů, poškozený vzorek
- Endogenní- druhý target kromě detekovaného genu, v multiplexu nebo zvlášť, standardizace množství DNA n RNA
- Exogenní- je známa exprese daného genu (předchozí reakce, plazmid....)
- Spike control

# Kontroly

## qPCR controls



### NEGATIVE

- No Template Control

### AIM

Detection of primers dimers and contamination

- No Amplification Control

Detection of probe's degradation

- No RT Control

Detection of genomic DNA contamination



### POSITIVE

- Endogenous Control  
(same sample, different target)

### AIM

Check quality of reagents.  
Also used for normalization.

- Exogenous Control  
(same target, different sample)

Check quality of reagents.

- Spiking Control  
(additional DNA spiked into the sample, different target)

Detect inhibitors presence  
Reject false negative in diagnostic assays

Figure 23. Summary of the main existing controls in qPCR and their interest.

# RT-qPCR

- Accuracy, sensitivity, fast results
- Monitoring of amplification in real-time

Bustin, 2010

# RT-PCR

- Experimental design
- RNA extraction
- RNA quality control
- Reverse transcription
- Primer and amplicon design
- qPCR validation
- Choice of reference genes
- Experimental reproducibility

# Experimental design

- mRNA transcription sensitive to external stimuli- need to minimize
- Define
  - procedures
  - control groups
  - type and number of replicates
  - experimental conditions- minimize variability

# RNA extraction

- From ‘fresh’ material if possible
- RNA stored at -80C or in RNA storage solution
- Minimize handling time- 10-20 samples
- DNase I treatment

# RNA quality control

- High purity (no contamination)
- High integrity (not degraded)
- Impurities- PCR inhibition
- Purity- protein contamination
- OD<sub>260/280</sub> 1.8-2.0 no protein
- OD<sub>260/230</sub> 1.8-2.0 no organic contaminants
- RIN>7
- Consistency in purity and integrity-reduction of variability of samples
- Immediately follow with procedures, store only cDNA

# Reverse Transcription

- Immediately after isolation- no degradation of RNA from freeze/thaw
- Consistent and complete coverage of transcribed regions
- Always enter same amount of RNA and same reaction time for all samples
- Ctrl
  - no RT samples (contamination with genomic DNA)
  - no template control (contamination)
- RT Buffer
  - mix of random primers
  - RNase H
  - RT enzyme- broad dynamic range

# Primer and amplicon design

- Essential for specific and efficient amplification
- Target sequences
  - Unique
  - 75-100 bp
  - GC content 50-60%
  - No secondary structures
- Primers
  - GC content 50-60%
  - Melting temperature 55-65C
  - No long stretches of G or C
  - G or C at the end of primer
  - Primer blast, MFOLD, experience

# qPCR validation

- Assessed for optimal range of primer annealing temperatures, efficiency, specificity using a standard set of samples
- Reaction conditions, buffers, primers optimized
- cDNA samples not contaminated
- [\*www.bio-rad.com/genomics/pcrsupport\*](http://www.bio-rad.com/genomics/pcrsupport)

# qPCR validation

- Optimal annealing T for primers- temperature gradient
- Analysis of PCR product- melt curve analysis (single sharp peak)
- Samples run on gel
- NTC necessary (primer –dimer, DNA contamination)

# PCR efficiency

- Measure of rate at which polymerase converts the reagents to amplicon
- Maximum increase per cycle is 2-fold – 100% efficiency
- Low efficiency
  - inhibitors of polymerase
  - high or suboptimal annealing temperature
  - old/inactive Taq
  - poorly designed primers
  - secondary structures

# Standard curve

- 10-fold dilution – 8 points
- Broad dynamic range
- For each point- in triplicates, get Ct values
- Need tight technical replicates
- If OK- Ct values separated by 3.32 cycles
- Need 90-110% Efficiency
- R values- how well data fit on curve
- $R^2 > 0.985$  OK
- Will define dynamic range of reaction

# qPCR

- Commercial qPCR kits
- Sample volumes- 10-50ul in 96 well plate format
- Software analysis
  - Flexibility in set up info
  - Group wells
  - Gene expression analysis
  - Ability to combine multiple plates

# Choice of reference genes

- Perfect reference gene- no expression changes between samples from various experimental conditions, time points
- How to find:
  - Extract RNA from 1-2 samples from each condition or time point, confirm purity and quality
  - Normalize concentration, do RT from same volume
  - Do qPCR from same volume of cDNA
  - geNorm method to calculate stability  
(*med-gen.ugent.be/genorm/*)
  - Need 3-5 genes

# Experimental reproducibility

- 2 sources of variability:
  - Biological- differences of organisms, tissues, cell cultures
  - Technical- pipetting, samples quality...
- 3 biological and 2 technical replicates
- 3 biological replicates- separate and independent experiments


# Key steps for qPCR

- Appropriate number of biological replicates and control samples
- Strict protocols for acquisition, processing and storage
- RNA purity and integrity
- Reverse Transcription
- Proper design of PCR

## Kvantitativní vztah mezi


množstvím PCR produktu (amplikonu) a intenzitou fluorescence

- Amplifikační práh detekce (Ct)

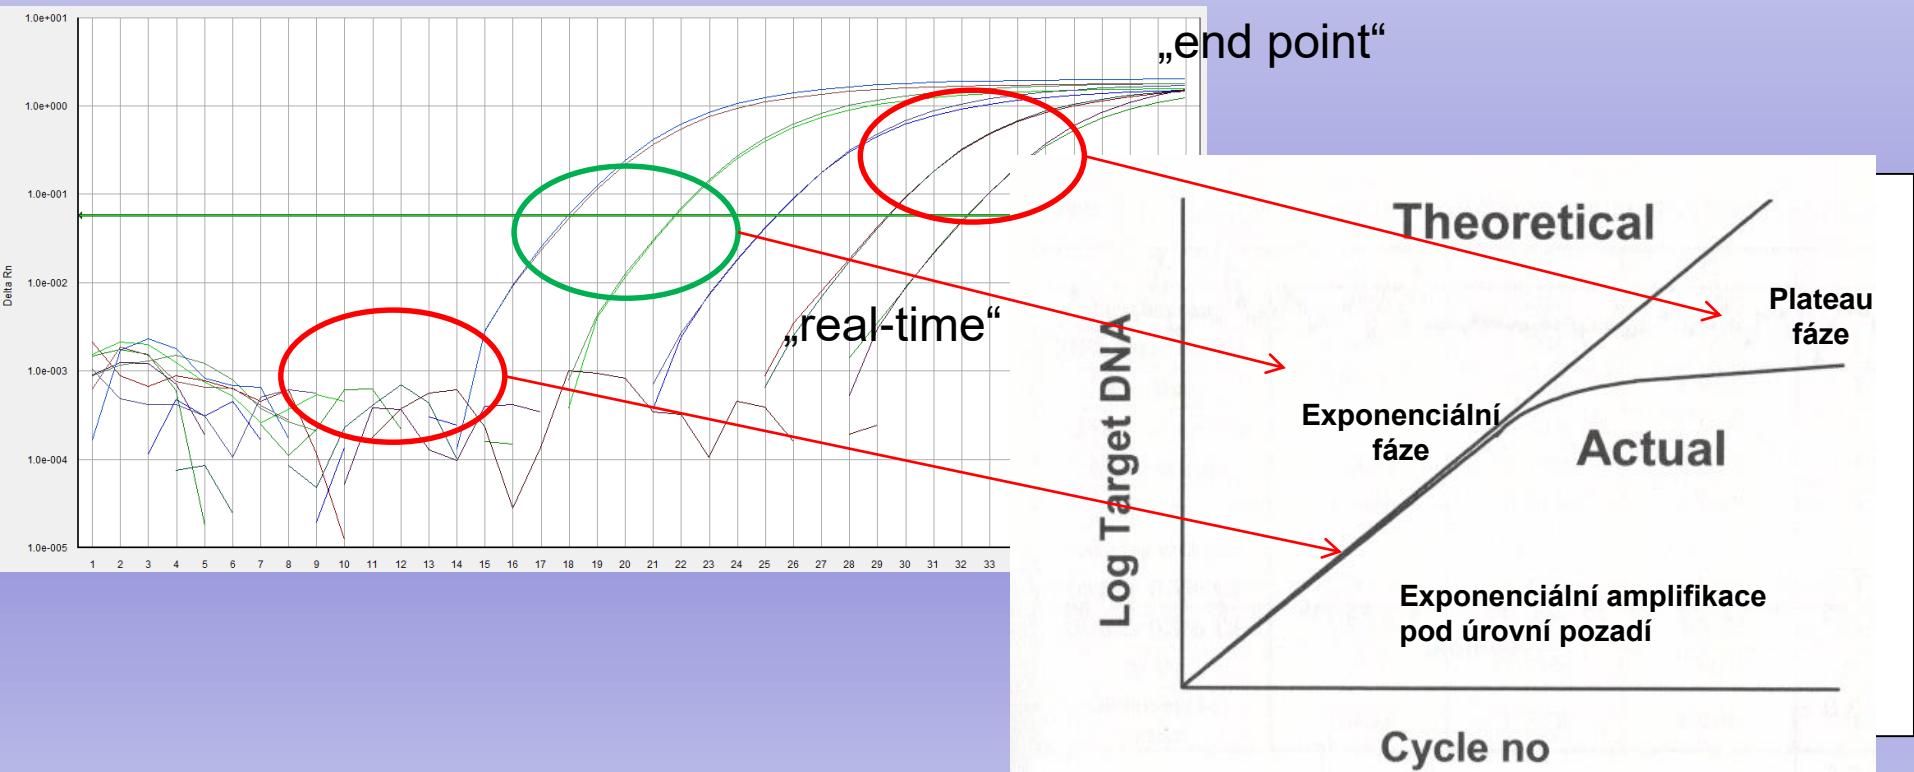


## Threshold cycle „Ct“

- určený na základě hodnoty fluorescence pozadí (background) a aktuální fluorescence vzorku
- kvantitativní výstup pro každý vzorek

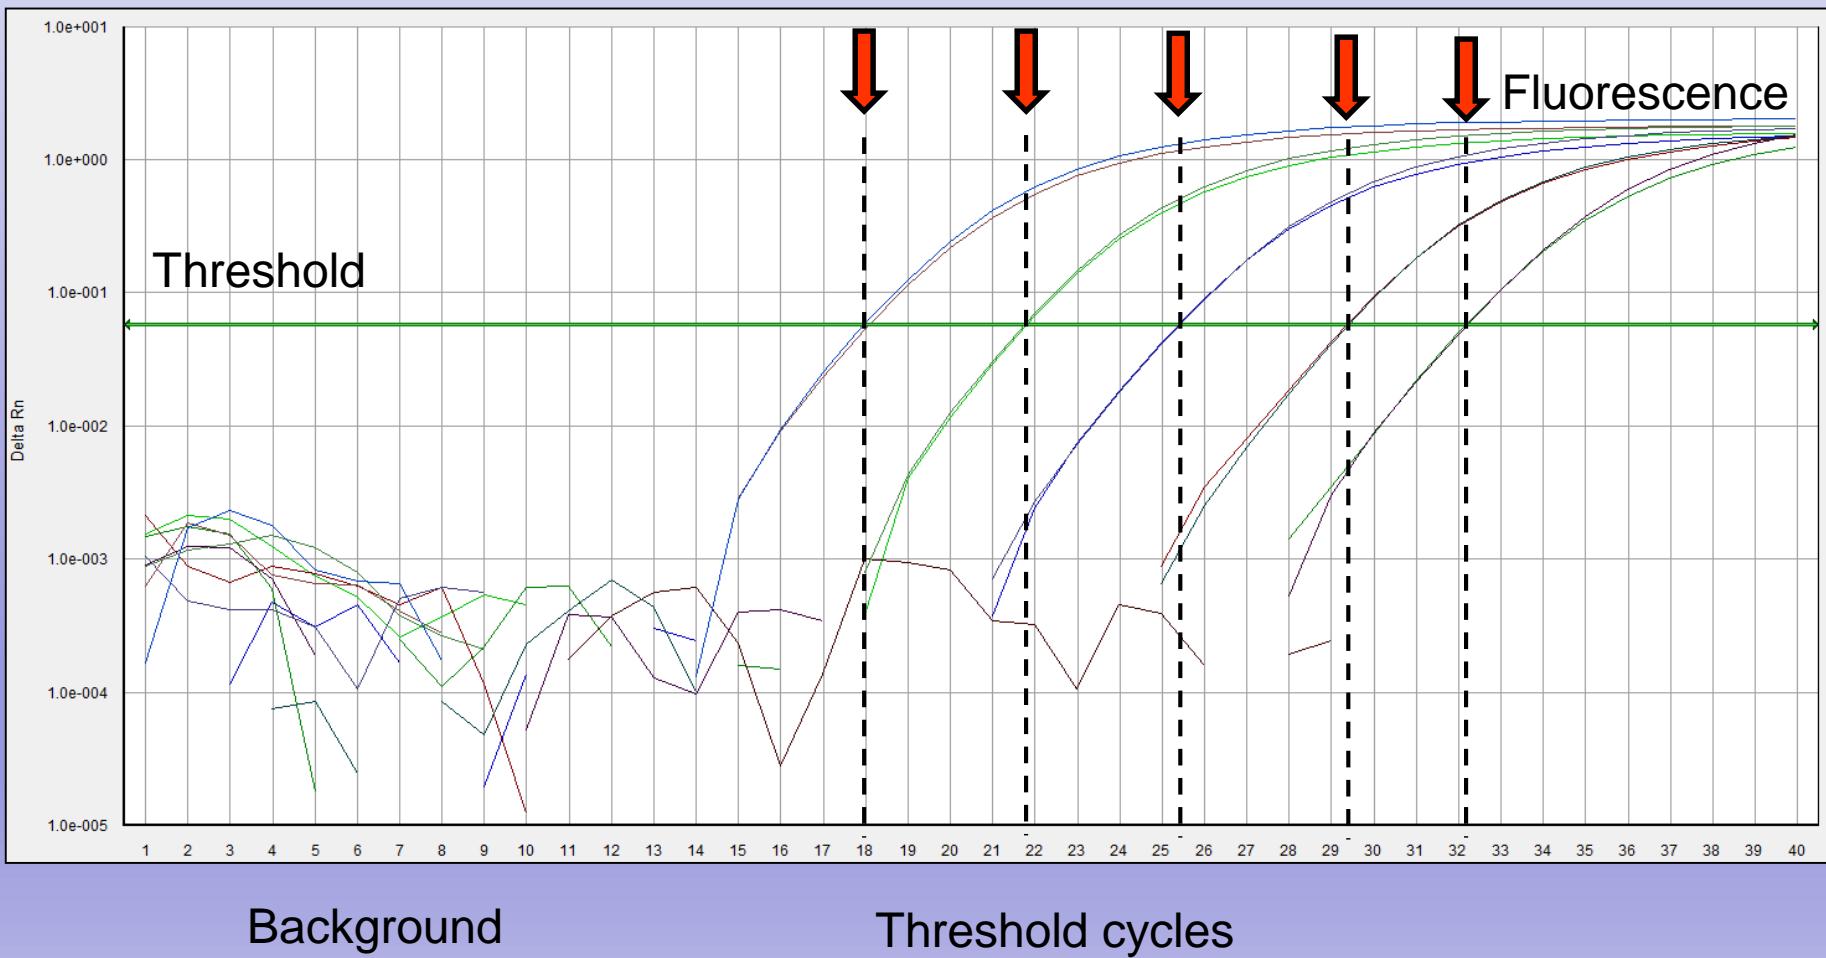

## Threshold cycle „Ct“

- počáteční množství kopií templátu
- definovaný v exponenciální fázi PCR
- stejná účinnost PCR ve všech reakcích
- účinnost štěpení fluorogenní sondy nebo vazby fluoroforu na DNA
- citlivost detekce
- čím menší Ct - tím větší počet kopií templátu na začátku reakce

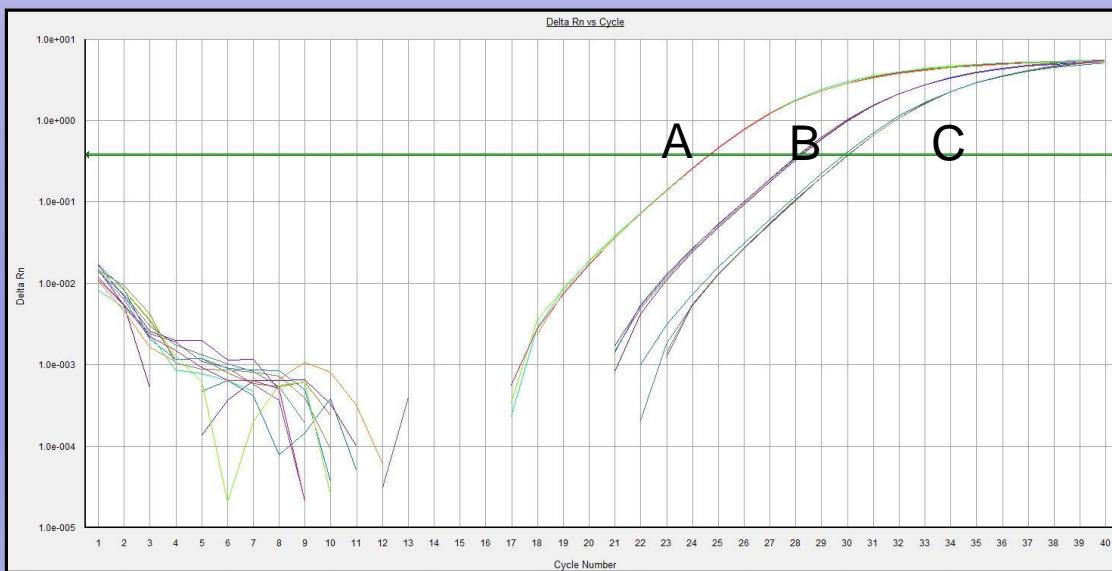

A > B > C

## Threshold cycle „Ct“

- rozdíl 1 Ct – dvojnásobné množství templátu


$$2^1 = 2$$

- kolika cyklům odpovídá odpovídá 10ti násobný rozdíl v množství templátu?

(předpokládáme 100% účinnost PCR)


$$2^n = 10$$

$$n=3,32$$

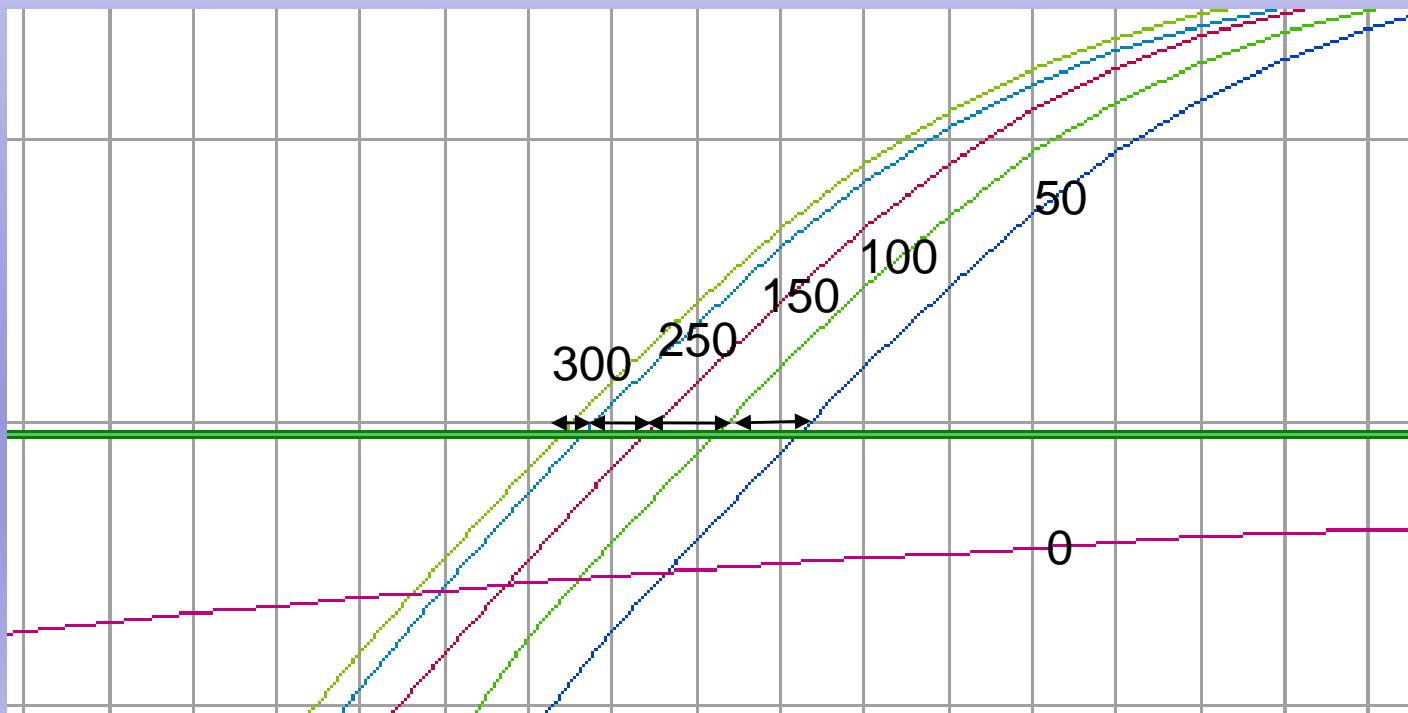


## Cross contamination



Vzorek 1



Vzorek 2



Vzájemná  
kontaminace  
vzorků




PCR 1


PCR 2

Přenos  
amplikonu do  
dalších PCR

## Carry-over contamination






PCR 1



PCR 2

## Jak předejít kontaminaci

- Správná laboratorní praxe
- Plastik v RNA kvalitě
- Automatizace

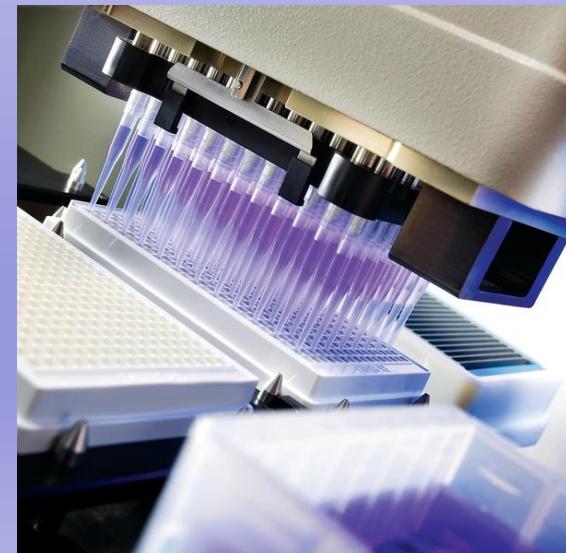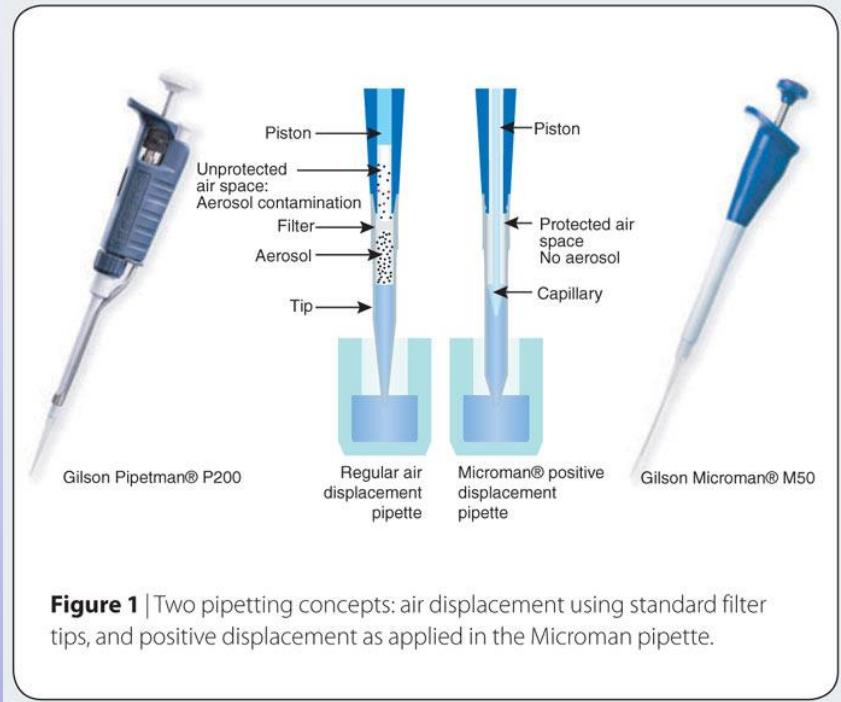

# Prevence kontaminace

- Fyzické oddělení pre a postPCR procesů
- Pipety a jiné nástroje oddělit
- Rukavice měnit často
- Reakci připravit v laminárním boxu
- Filtrované špičky
- Reagencie – pracovat opatrně, zabránit kontaminaci
- UV světlo pro dekontaminaci místnosti, 10% savo

# Nejčastější důvody špatné PCR

- Špatný design primerů a sond
- Špatná kvalita RNA
- Nepoužívání master mixů
- Cross-contamination
- Nepoužití no RT control (NAC ctrl)
- Špatná normalizační kontrola
- Sybr green – melting curve
- Ct cycle – v exponenciální oblasti
- Špatná efektivita reakce
- Špatně udělaná standardní křivky

# Co je sonda

- qPCR založeno na detekci fluorescenčního signálu
  - Taqman probes (FRET)
  - Molecular beacons (FRET)
  - Scorpions (FRET)
  - Sybr green
- Detekce PCR produktů vyrobením fluorescenčního signálu

# Co jsou primery

- Sekvenčně specifické úseky DNA